
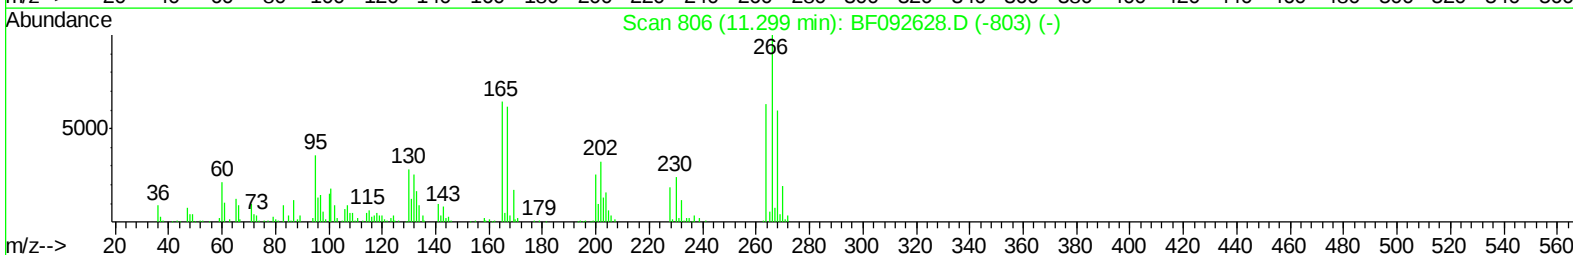
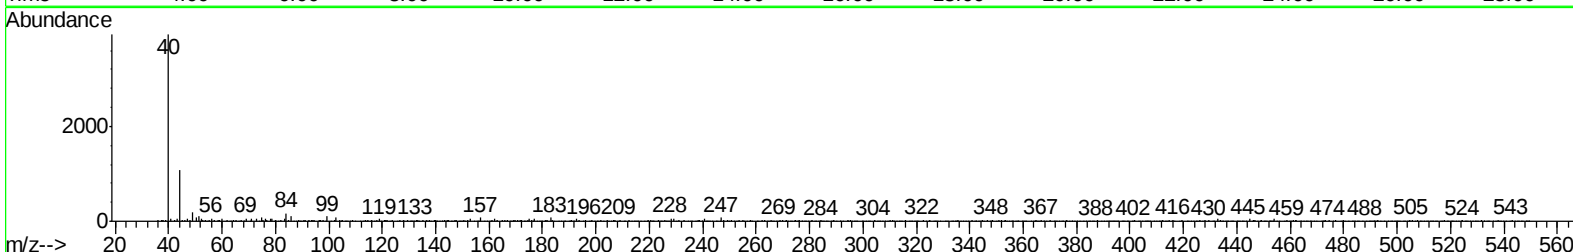


Data File : BE092745.D
Acq On : 20 Feb 2017 13:29
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 01:04:33 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

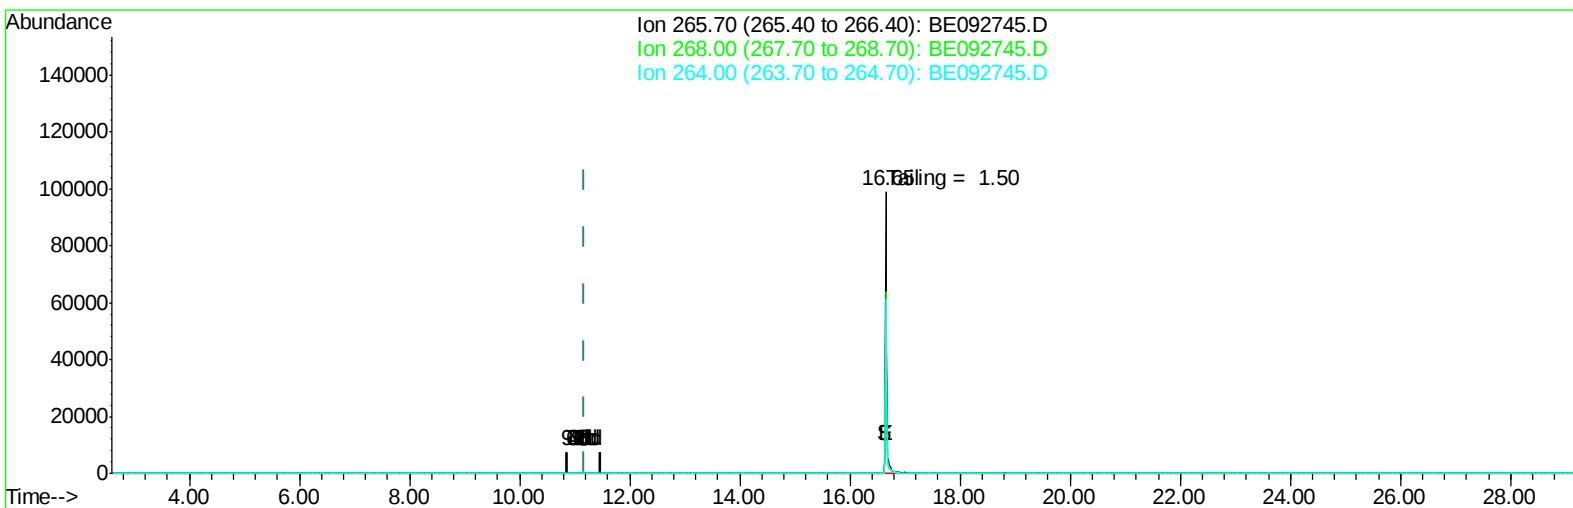

TIC: BE092745.D




(69) Pentachlorophenol (C)
11.154min (-0.031) 116.47ng

response 16

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	192.86#
264.00	62.90	28.57#
0.00	0.00	0.00

Data File : BE092745.D
Acq On : 20 Feb 2017 13:29
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 01:04:33 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

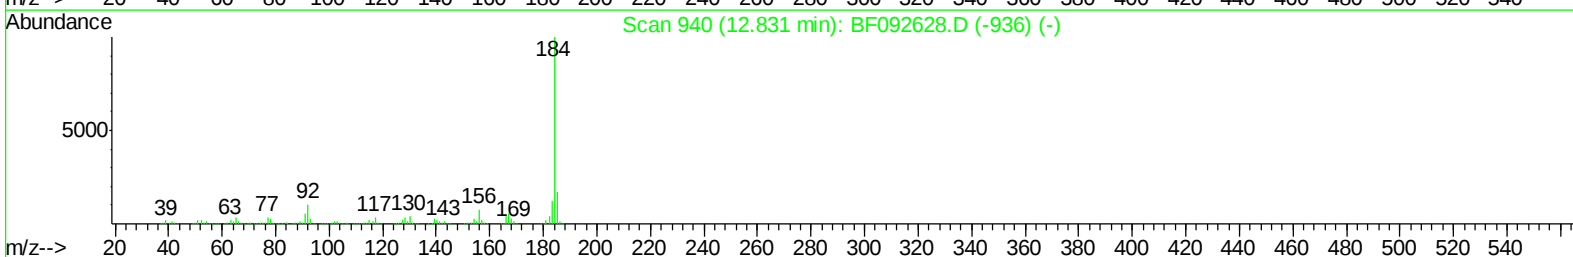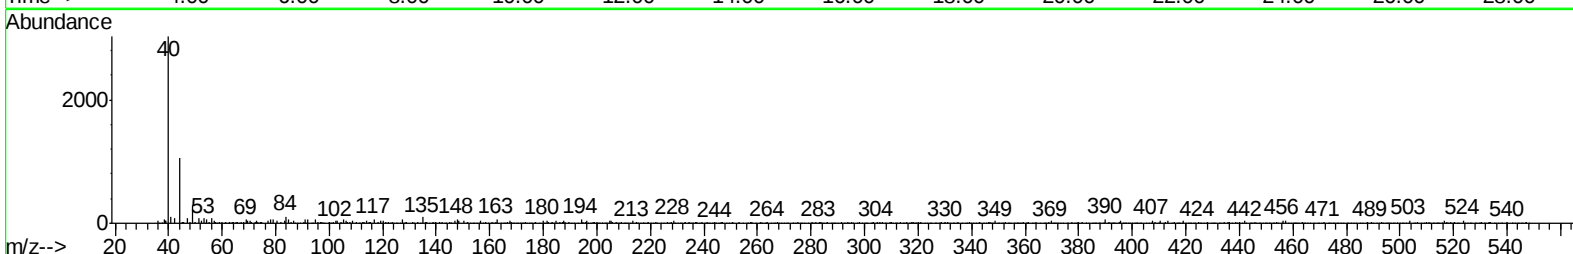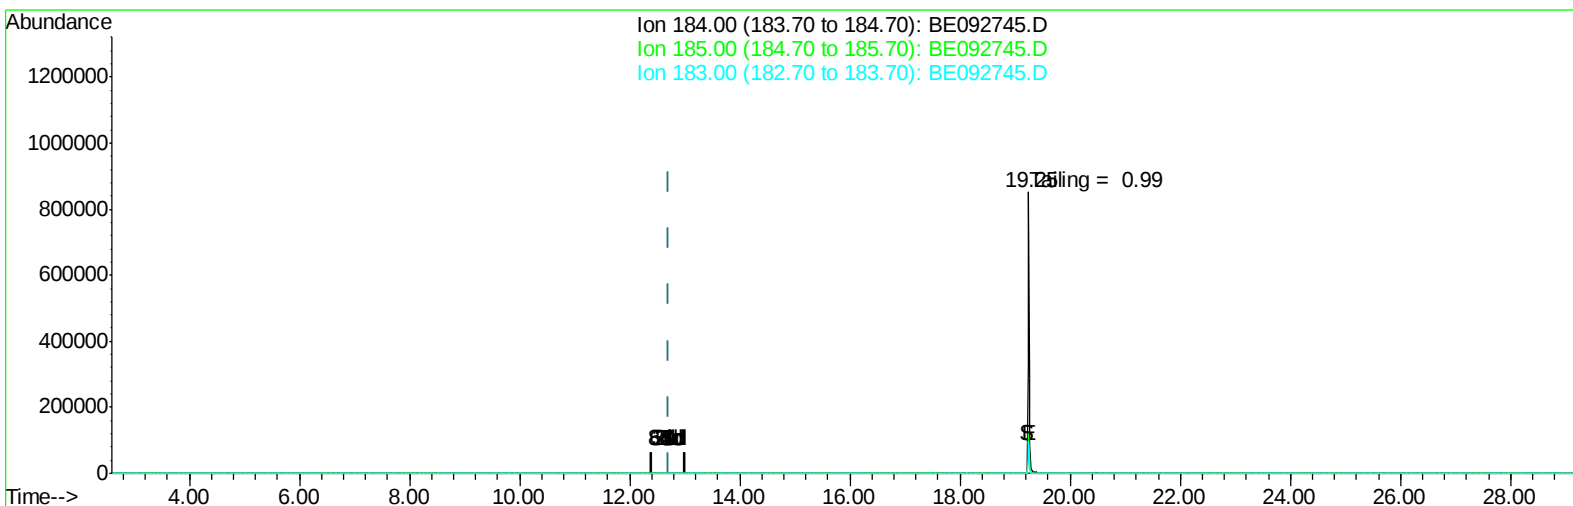

TIC: BE092745.D

(76) Benzidine

12.706min (-0.011) 239.37ng

response 51

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	13.04#
183.00	11.50	41.30#
0.00	0.00	0.00