


Data Path : Z:\HPCHEM1\BNA_E\Data\BE022017\
 Data File : BE092745.D
 Acq On : 20 Feb 2017 13:29
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE021517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 15 17:05:20 2017

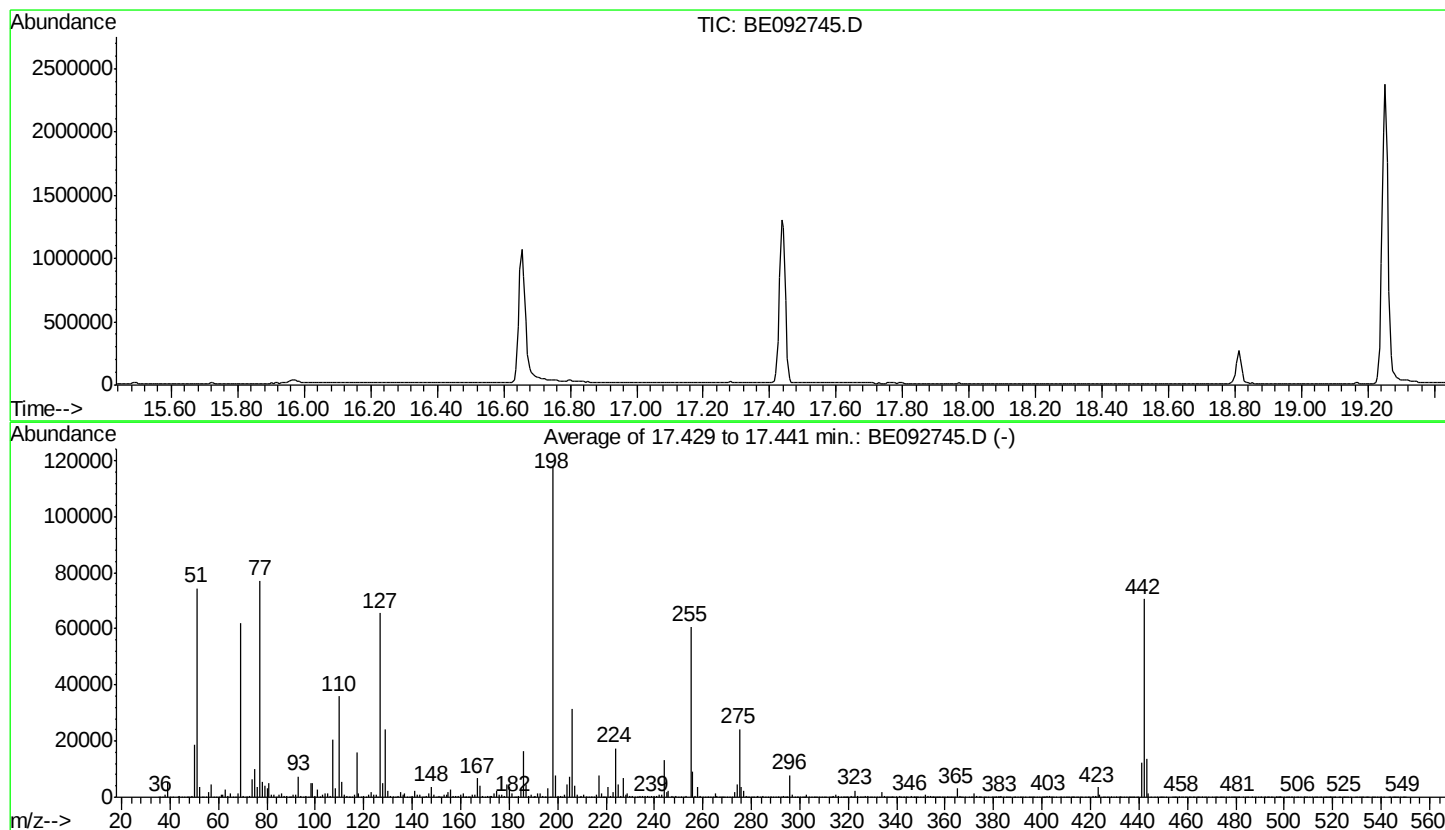

AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.0	74426	PASS
68	69	0.00	2	1.9	1187	PASS
69	198	0.00	100	52.4	61881	PASS
70	69	0.00	2	0.6	347	PASS
127	198	10	80	55.4	65498	PASS
197	198	0.00	2	0.2	231	PASS
198	198	100	100	100.0	118169	PASS
199	198	5	9	6.7	7961	PASS
275	198	10	60	20.6	24314	PASS
365	198	1	100	2.7	3143	PASS
441	442	0.01	24	17.6	12385	PASS
442	198	50	100	59.7	70522	PASS
443	442	15	24	19.6	13855	PASS