
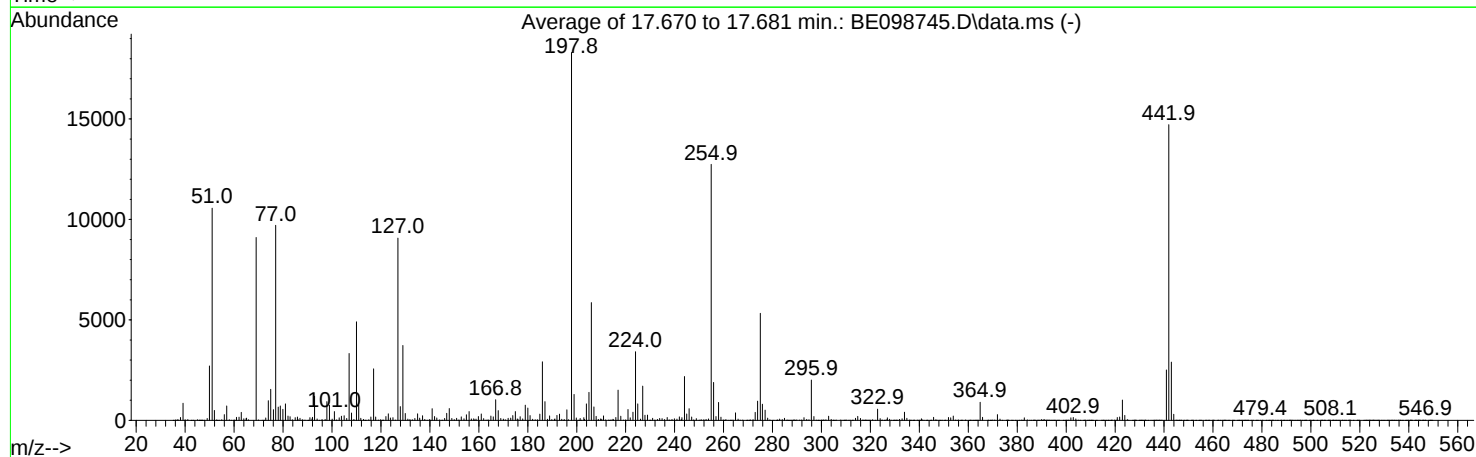


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE022119\
 Data File : BE098745.D
 Acq On : 21 Feb 2019 12:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 24 14:44:44 2019

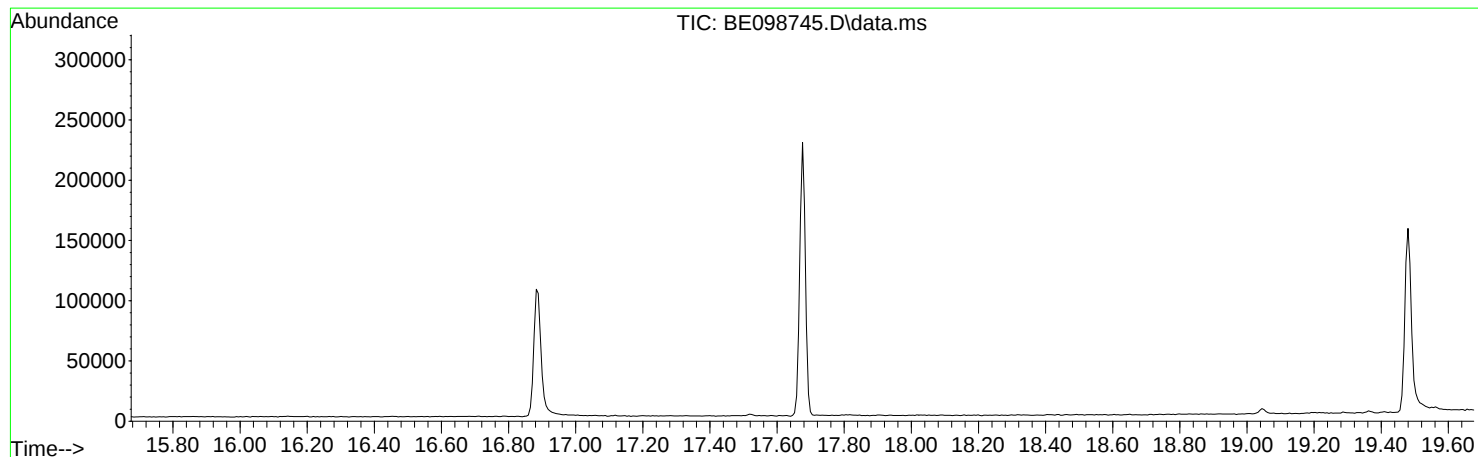

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.7	10556	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.7	9101	PASS
70	69	0.00	2	0.3	27	PASS
127	198	10	80	49.5	9071	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18309	PASS
199	198	5	9	7.1	1291	PASS
275	198	10	60	29.1	5327	PASS
365	198	1	100	4.9	904	PASS
441	198	0.01	100	13.7	2508	PASS
442	198	50	100	80.4	14717	PASS
443	442	15	24	19.7	2901	PASS