

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE022315\
 Data File : BE089655.D
 Acq On : 24 Feb 2015 00:08
 Operator : TP/JJ
 Sample : SSTDICC010
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 24 03:18:31 2015

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 24 03:06:59 2015

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.34	152	41514	5.00	ng	0.00
4) Naphthalene-d8	12.24	136	174554	5.00	ng	0.00
8) Acenaphthene-d10	16.42	164	77596	5.00	ng	0.00
13) Phenanthrene-d10	19.77	188	143038	5.00	ng	0.00
19) Chrysene-d12	23.66	240	126892	5.00	ng	0.00
25) Perylene-d12	25.34	264	102981	5.00	ng	0.00

System Monitoring Compounds

5) Nitrobenzene-d5	10.61	82	107808	13.57	ng	0.00
9) 2-Fluorobiphenyl	14.88	172	174955	8.64	ng	0.00
21) Terphenyl-d14	22.30	244	159227	7.80	ng	0.00


Target Compounds


						Qvalue
2) 1,4-Dioxane	2.69	88	50257	7.32	ng	98
3) n-Nitrosodimethylamine	3.32	42	75071	10.26	ng	96
6) Naphthalene	12.29	128	336901	8.50	ng	99
7) 2-Methylnaphthalene	13.95	142	208005	9.32	ng	98
10) Acenaphthylene	16.07	152	1241473	9.66	ng	100
11) Acenaphthene	16.50	154	181368	8.81	ng	98
12) Fluorene	17.74	166	205623	9.56	ng	99
14) Hexachlorobenzene	19.00	284	38440	8.69	ng	97
15) Pentachlorophenol	19.44	266	11077	10.10	ng	93
16) Phenanthrene	19.81	178	307308	8.57	ng	100
17) Anthracene	19.91	178	299066	10.31	ng	99
18) Fluoranthene	21.72	202	295862	11.38	ng	100
20) Pyrene	22.04	202	317327	7.96	ng	99
22) Benzo(a)anthracene	23.64	228	1034903	11.11	ng	95
23) Chrysene	23.68	228	1099334	7.99	ng	93
24) Indeno(1,2,3-cd)pyrene	26.75	276	882359	17.05	ng	# 90
26) Benzo(b)fluoranthene	24.91	252	192193	19.50	ng	97
27) Benzo(k)fluoranthene	24.94	252	284507	11.00	ng	98
28) Benzo(a)pyrene	25.27	252	192807	16.96	ng	97
29) Dibenzo(a,h)anthracene	26.78	278	173706	18.20	ng	94
30) Benzo(g,h,i)perylene	27.17	276	747294	12.64	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE022315\
Data File : BE089655.D
Acq On : 24 Feb 2015 00:08
Operator : TP/JJ
Sample : SSTDICC010
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Feb 24 03:18:31 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 24 03:06:59 2015
Response via : Initial Calibration





#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 9.34 min Scan# 1299

Delta R.T. 0.00 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08


Tgt Ion: 152 Resp: 41514

Ion Ratio Lower Upper

152 100

150 155.1 127.0 190.6




115 63.6 52.4 78.6



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E



#2

1,4-Dioxane

Concen: 7.32 ng

RT: 2.69 min Scan# 191

Delta R.T. -0.01 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08


Tgt Ion: 88 Resp: 50257

Ion Ratio Lower Upper

88 100

58 78.6 61.8 92.6



43 34.6 26.4 39.6




Abundance Ion 88.00 (87.70 to 88.70): BE0

Ion 58.00 (57.70 to 58.70): BE0

Ion 43.00 (42.70 to 43.70): BE0









#3

n-Nitrosodimethylamine
 Concen: 10.26 ng
 RT: 3.32 min Scan# 284
 Delta R.T. -0.05 min
 Lab File: BE089655.D
 Acq: 24 Feb 2015 00:08

Tgt Ion: 42 Resp: 75071
 Ion Ratio Lower Upper
 42 100
 74 110.9 92.5 138.7
 44 5.6 4.9 7.3




Abundance Ion 42.00 (41.70 to 42.70): BE0
 Ion 74.00 (73.70 to 74.70): BE0
 Ion 44.00 (43.70 to 44.70): BE0

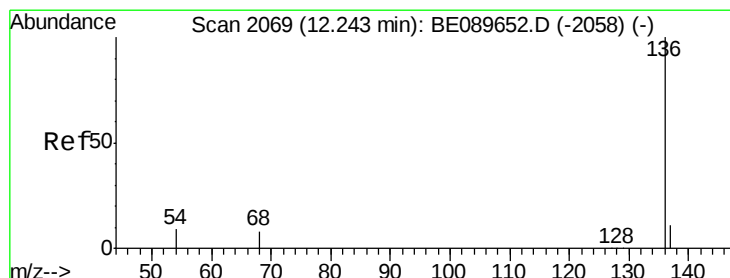



#4


Naphthalene-d8
 Concen: 5.00 ng
 RT: 12.24 min Scan# 2069
 Delta R.T. -0.00 min
 Lab File: BE089655.D
 Acq: 24 Feb 2015 00:08

Tgt Ion: 136 Resp: 174554
 Ion Ratio Lower Upper
 136 100
 137 10.8 8.7 13.1
 54 10.7 7.5 11.3



Abundance Ion 136.00 (135.70 to 136.70): E
 Ion 137.00 (136.70 to 137.70): E
 Ion 54.00 (53.70 to 54.70): BE0





#5

Nitrobenzene-d5

Concen: 13.57 ng

RT: 10.61 min Scan# 1668


Delta R.T. 0.00 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08

Tgt Ion: 82 Resp: 107808

Ion	Ratio	Lower	Upper
82	100		
128	41.6	31.0	46.4
54	53.9	43.8	65.8






Abundance

Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0



#6

Naphthalene

Concen: 8.50 ng

RT: 12.29 min Scan# 2078


Delta R.T. -0.00 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08

Tgt Ion: 128 Resp: 336901

Ion	Ratio	Lower	Upper
128	100		
129	11.0	8.8	13.2
127	12.7	9.8	14.6





Abundance

Ion 128.00 (127.70 to 128.70): BE0

Ion 129.00 (128.70 to 129.70): BE0

Ion 127.00 (126.70 to 127.70): BE0





#7

2-Methylnaphthalene

Concen: 9.32 ng





RT: 13.95 min Scan# 2417

Delta R.T. 0.00 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08

Tgt Ion:	142	Resp:	208005
Ion Ratio	Lower	Upper	
142	100		
141	84.2	68.6	103.0
115	34.8	29.0	43.6



#8

Acenaphthene-d10

Concen: 5.00 ng




RT: 16.42 min Scan# 2852

Delta R.T. 0.00 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08





Tgt Ion:	164	Resp:	77596
Ion Ratio	Lower	Upper	
164	100		
162	95.7	75.4	113.2
160	43.1	33.7	50.5








#9
2-Fluorobiphenyl
Concen: 8.64 ng
RT: 14.88 min Scan# 2621
Delta R.T. -0.00 min
Lab File: BE089655.D
Acq: 24 Feb 2015 00:08


Tgt Ion	Ratio	Lower	Upper
172	100		
171	33.9	26.2	39.4
170	22.8	17.7	26.5

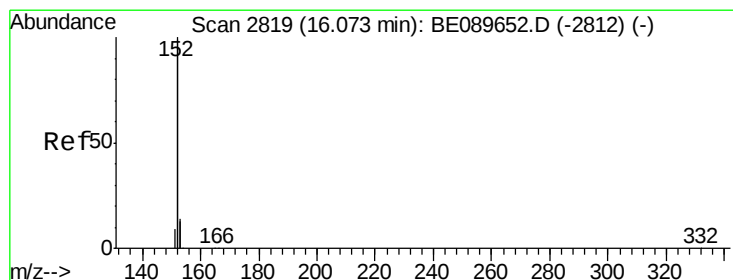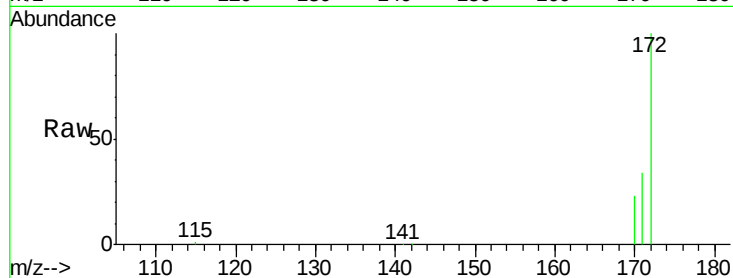

#10
Acenaphthylene
Concen: 9.66 ng
RT: 16.07 min Scan# 2820
Delta R.T. 0.00 min
Lab File: BE089655.D
Acq: 24 Feb 2015 00:08

Tgt Ion	Ratio	Lower	Upper
152	100		
151	4.8	3.8	5.6
153	13.1	10.4	15.6





#11

Acenaphthene

Concen: 8.81 ng

RT: 16.50 min Scan# 2859

Delta R.T. 0.01 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08


Tgt Ion:154 Resp: 181368

Ion Ratio Lower Upper

154 100

153 424.8 343.0 514.4




152 204.6 165.8 248.8



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E



#12

Fluorene

Concen: 9.56 ng

RT: 17.74 min Scan# 2972

Delta R.T. 0.00 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08


Tgt Ion:166 Resp: 205623

Ion Ratio Lower Upper

166 100

165 92.7 73.6 110.4



167 13.3 10.5 15.7




Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E


Ion 167.00 (166.70 to 167.70): E








#13
Phenanthrene-d10
Concen: 5.00 ng
RT: 19.77 min Scan# 3176
Delta R.T. 0.01 min
Lab File: BE089655.D
Acq: 24 Feb 2015 00:08

Tgt Ion:188 Resp: 143038
Ion Ratio Lower Upper
188 100
94 12.4 13.8 20.8#
80 12.7 15.0 22.6#




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0






#14
Hexachlorobenzene
Concen: 8.69 ng
RT: 19.00 min Scan# 3090
Delta R.T. 0.01 min
Lab File: BE089655.D
Acq: 24 Feb 2015 00:08

Tgt Ion:284 Resp: 38440
Ion Ratio Lower Upper
284 100
142 66.4 55.0 82.6
249 30.3 26.1 39.1




Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E








#15
 Pentachlorophenol
 Concen: 10.10 ng
 RT: 19.44 min Scan# 3139
 Delta R.T. 0.01 min
 Lab File: BE089655.D
 Acq: 24 Feb 2015 00:08

Tgt Ion: 266 Resp: 11077
 Ion Ratio Lower Upper
 266 100
 268 66.2 54.7 82.1
 264 60.7 55.4 83.0




Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 268.00 (267.70 to 268.70): E
 Ion 264.00 (263.70 to 264.70): E






#16
 Phenanthrene
 Concen: 8.57 ng
 RT: 19.81 min Scan# 3180
 Delta R.T. -0.00 min
 Lab File: BE089655.D
 Acq: 24 Feb 2015 00:08

Tgt Ion: 178 Resp: 307308
 Ion Ratio Lower Upper
 178 100
 176 19.2 15.3 22.9
 179 15.4 12.3 18.5







Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E








#17
 Anthracene
 Concen: 10.31 ng
 RT: 19.91 min Scan# 3191
 Delta R.T. -0.00 min
 Lab File: BE089655.D
 Acq: 24 Feb 2015 00:08


Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.6	14.3	21.5
179	15.4	12.1	18.1

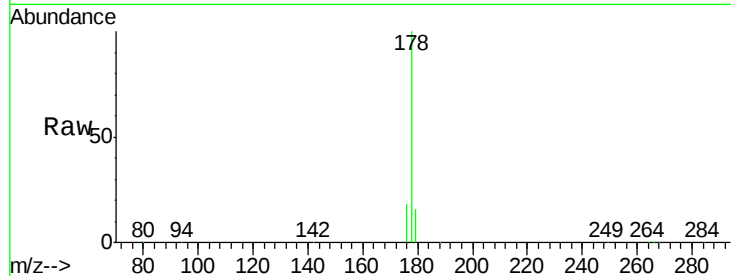

#18
 Fluoranthene
 Concen: 11.38 ng
 RT: 21.72 min Scan# 3476
 Delta R.T. -0.00 min
 Lab File: BE089655.D
 Acq: 24 Feb 2015 00:08


Tgt Ion	Ratio	Lower	Upper
202	100		
101	18.5	14.9	22.3
203	17.4	13.7	20.5








#19
Chrysene-d12
Concen: 5.00 ng
RT: 23.66 min Scan# 3807
Delta R.T. 0.00 min
Lab File: BE089655.D
Acq: 24 Feb 2015 00:08

Tgt Ion: 240 Resp: 126892
Ion Ratio Lower Upper
240 100
120 13.2 10.6 15.8
236 25.6 20.3 30.5




Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E






#20
Pyrene
Concen: 7.96 ng
RT: 22.04 min Scan# 3535
Delta R.T. -0.00 min
Lab File: BE089655.D
Acq: 24 Feb 2015 00:08

Tgt Ion: 202 Resp: 317327
Ion Ratio Lower Upper
202 100
200 20.9 16.5 24.7
203 17.7 13.8 20.6







Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E



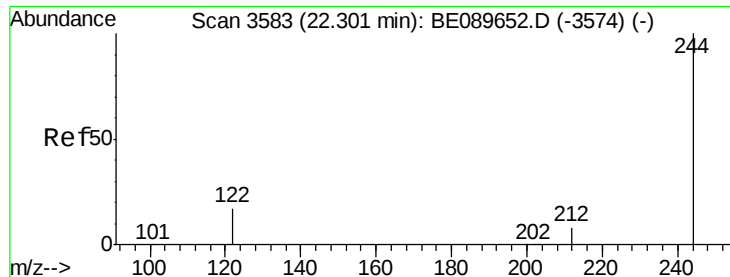




#21
 Terphenyl-d14
 Concen: 7.80 ng
 RT: 22.30 min Scan# 3585
 Delta R.T. -0.00 min
 Lab File: BE089655.D
 Acq: 24 Feb 2015 00:08

Tgt Ion: 244 Resp: 159227
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.6 10.0
 122 15.4 13.7 20.5

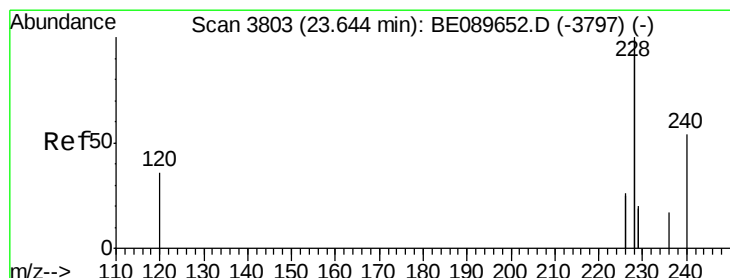

#22
 Benzo(a)anthracene
 Concen: 11.11 ng
 RT: 23.64 min Scan# 3804
 Delta R.T. -0.01 min
 Lab File: BE089655.D
 Acq: 24 Feb 2015 00:08

Tgt Ion: 228 Resp: 1034903
 Ion Ratio Lower Upper
 228 100
 226 29.0 20.9 31.3
 229 18.2 15.8 23.6





#23

Chrysene

Concen: 7.99 ng

RT: 23.68 min Scan# 3811

Delta R.T. -0.01 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08


Tgt Ion: 228 Resp: 1099334

Ion Ratio Lower Upper

228 100

226 31.9 22.0 33.0




229 17.8 16.6 24.8



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

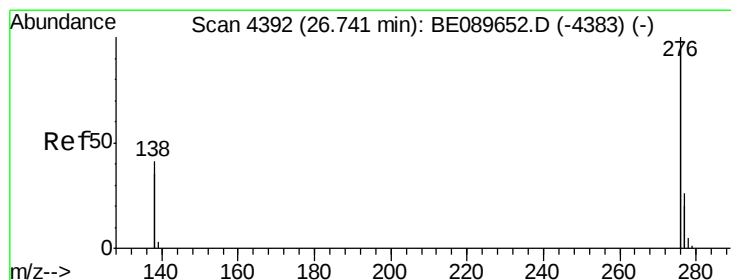

#24

Indeno(1,2,3-cd)pyrene

Concen: 17.05 ng

RT: 26.75 min Scan# 4395

Delta R.T. 0.01 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08


Tgt Ion: 276 Resp: 882359

Ion Ratio Lower Upper

276 100

138 43.0 36.2 54.4



277 25.0 5.4 8.2#




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E





Ion 277.00 (276.70 to 277.70): E



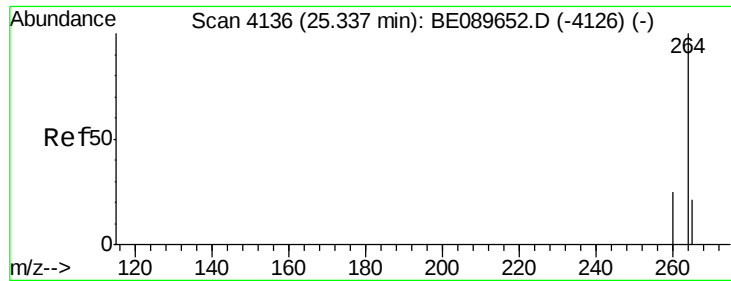




#25
 Perylene-d12
 Concen: 5.00 ng
 RT: 25.34 min Scan# 4137
 Delta R.T. -0.00 min
 Lab File: BE089655.D
 Acq: 24 Feb 2015 00:08


Tgt Ion: 264 Resp: 102981
 Ion Ratio Lower Upper
 264 100
 260 24.8 20.0 30.0
 265 21.0 16.8 25.2

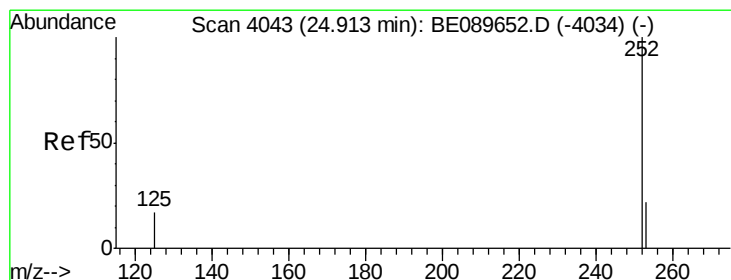

#26
 Benzo(b)fluoranthene
 Concen: 19.50 ng
 RT: 24.91 min Scan# 4044
 Delta R.T. -0.00 min
 Lab File: BE089655.D
 Acq: 24 Feb 2015 00:08





Tgt Ion: 252 Resp: 192193
 Ion Ratio Lower Upper
 252 100
 253 21.9 18.3 27.5
 125 16.5 14.6 22.0








#27
Benzo(k)fluoranthene
Concen: 11.00 ng
RT: 24.94 min Scan# 4050
Delta R.T. -0.00 min
Lab File: BE089655.D
Acq: 24 Feb 2015 00:08


Tgt Ion: 252 Resp: 284507
Ion Ratio Lower Upper
252 100
253 21.2 17.8 26.8
125 17.3 14.3 21.5



#28
Benzo(a)pyrene
Concen: 16.96 ng
RT: 25.27 min Scan# 4123
Delta R.T. -0.00 min
Lab File: BE089655.D
Acq: 24 Feb 2015 00:08

Tgt Ion: 252 Resp: 192807
Ion Ratio Lower Upper
252 100
253 21.6 18.4 27.6
125 18.4 15.9 23.9





#29

Dibenzo(a,h)anthracene

Concen: 18.20 ng

RT: 26.78 min Scan# 4399

Delta R.T. 0.00 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08


Tgt Ion: 278 Resp: 173706

Ion Ratio Lower Upper




278 100

139 26.6 25.4 38.2

279 24.0 20.0 30.0



Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E



#30

Benzo(g,h,i)perylene

Concen: 12.64 ng

RT: 27.17 min Scan# 4459

Delta R.T. 0.01 min

Lab File: BE089655.D

Acq: 24 Feb 2015 00:08


Tgt Ion: 276 Resp: 747294

Ion Ratio Lower Upper

276 100

277 24.3 20.2 30.2

138 35.8 32.4 48.6



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 277.00 (276.70 to 277.70): E
Ion 138.00 (137.70 to 138.70): E

