


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE022315\
Data File : BE089665.D
Acq On : 24 Feb 2015 7:15
Operator : TP/JJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 24 03:46:57 2015

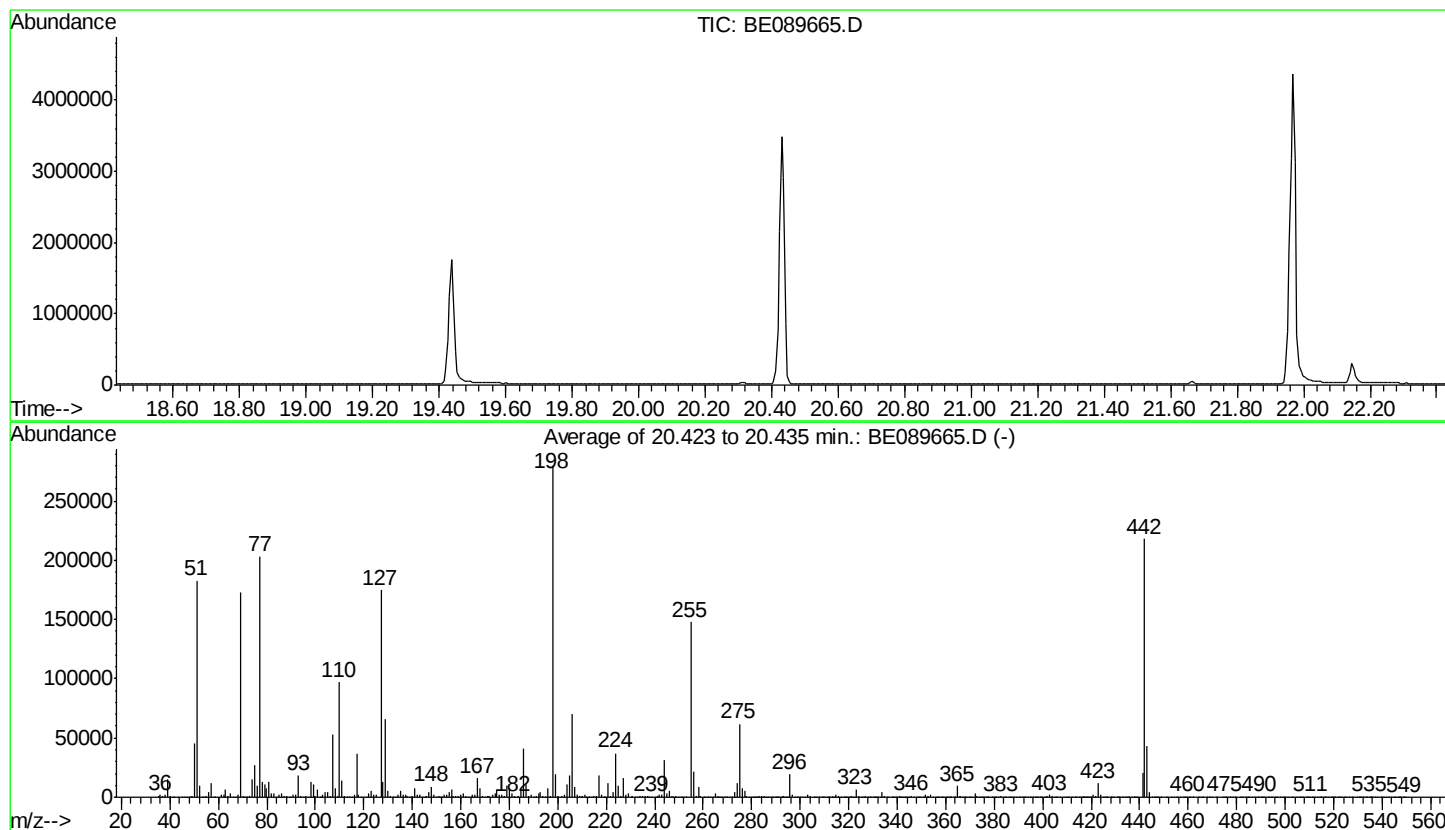

AutoFind: Scans 3240, 3241, 3242; Background Corrected with Scan 3232

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.4	183030	PASS
68	69	0.00	2	1.2	2145	PASS
69	198	0.00	100	61.7	172705	PASS
70	69	0.00	2	0.4	769	PASS
127	198	10	80	62.5	174928	PASS
197	198	0.00	2	0.3	810	PASS
198	198	100	100	100.0	279808	PASS
199	198	5	9	7.1	19752	PASS
275	198	10	60	22.0	61582	PASS
365	198	1	100	3.4	9631	PASS
441	442	0.01	24	9.2	20029	PASS
442	198	50	100	77.9	217893	PASS
443	442	15	24	19.8	43238	PASS