



n-Nitrosodimethylamine

Response Ratio

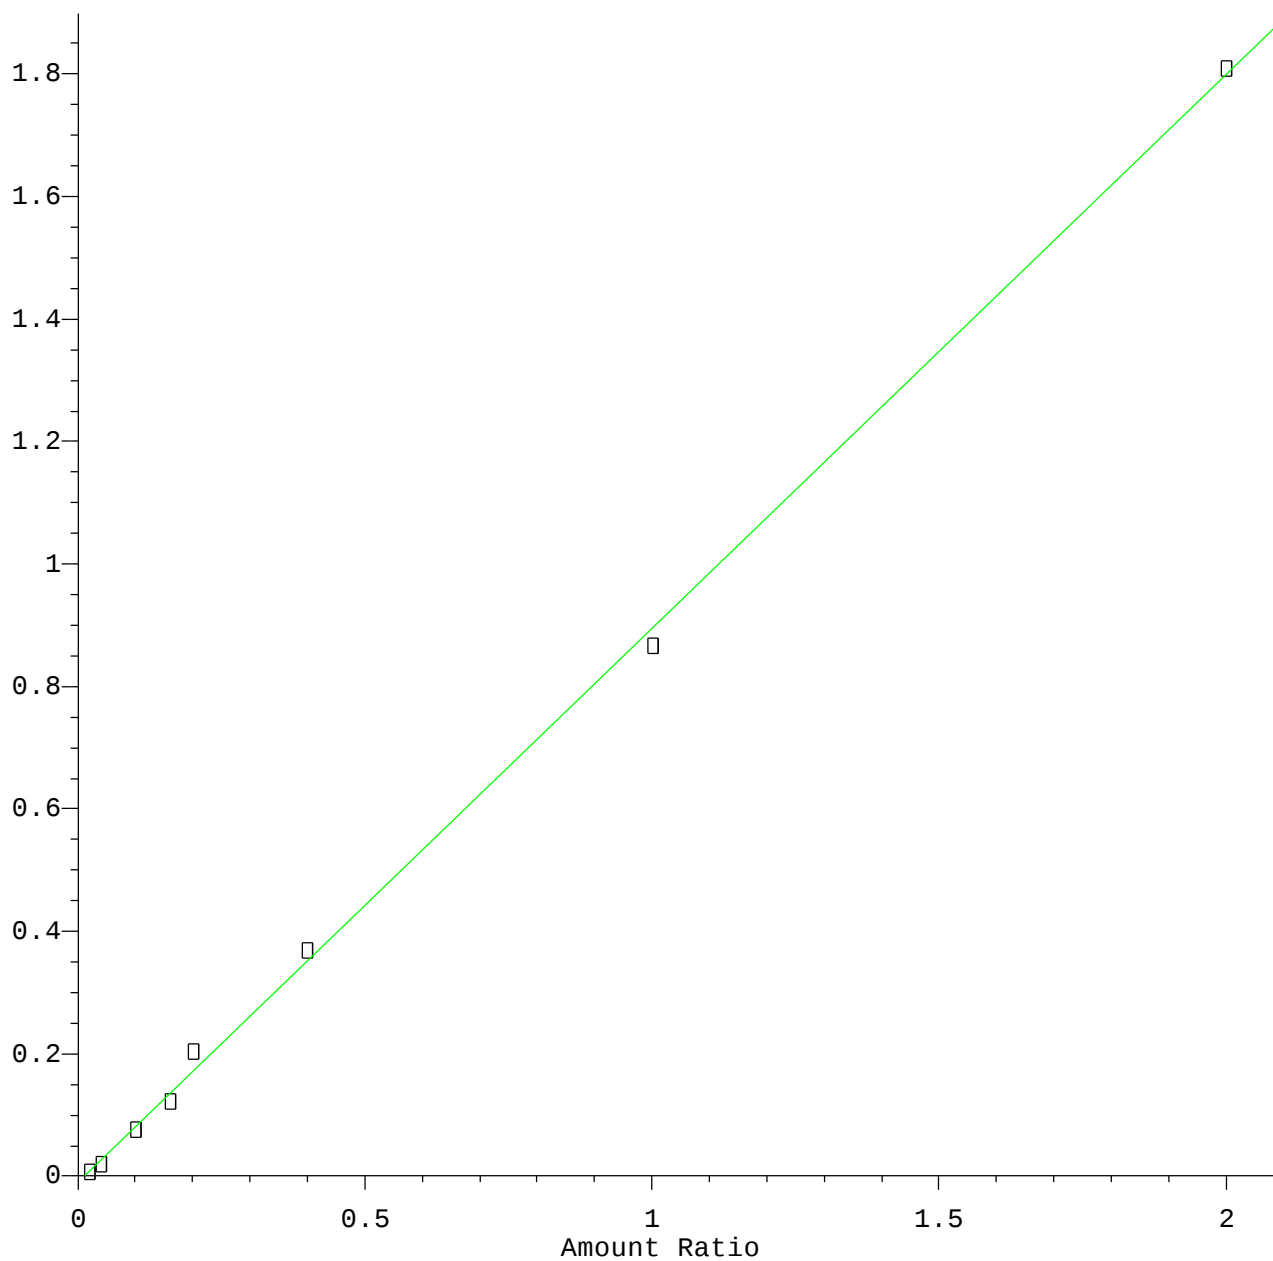


Resp Ratio = $9.05 \times 10^{-1} \times \text{Amt} - 1.02 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Calibration Table Last Updated: Tue Feb 24 03:37:34 2015

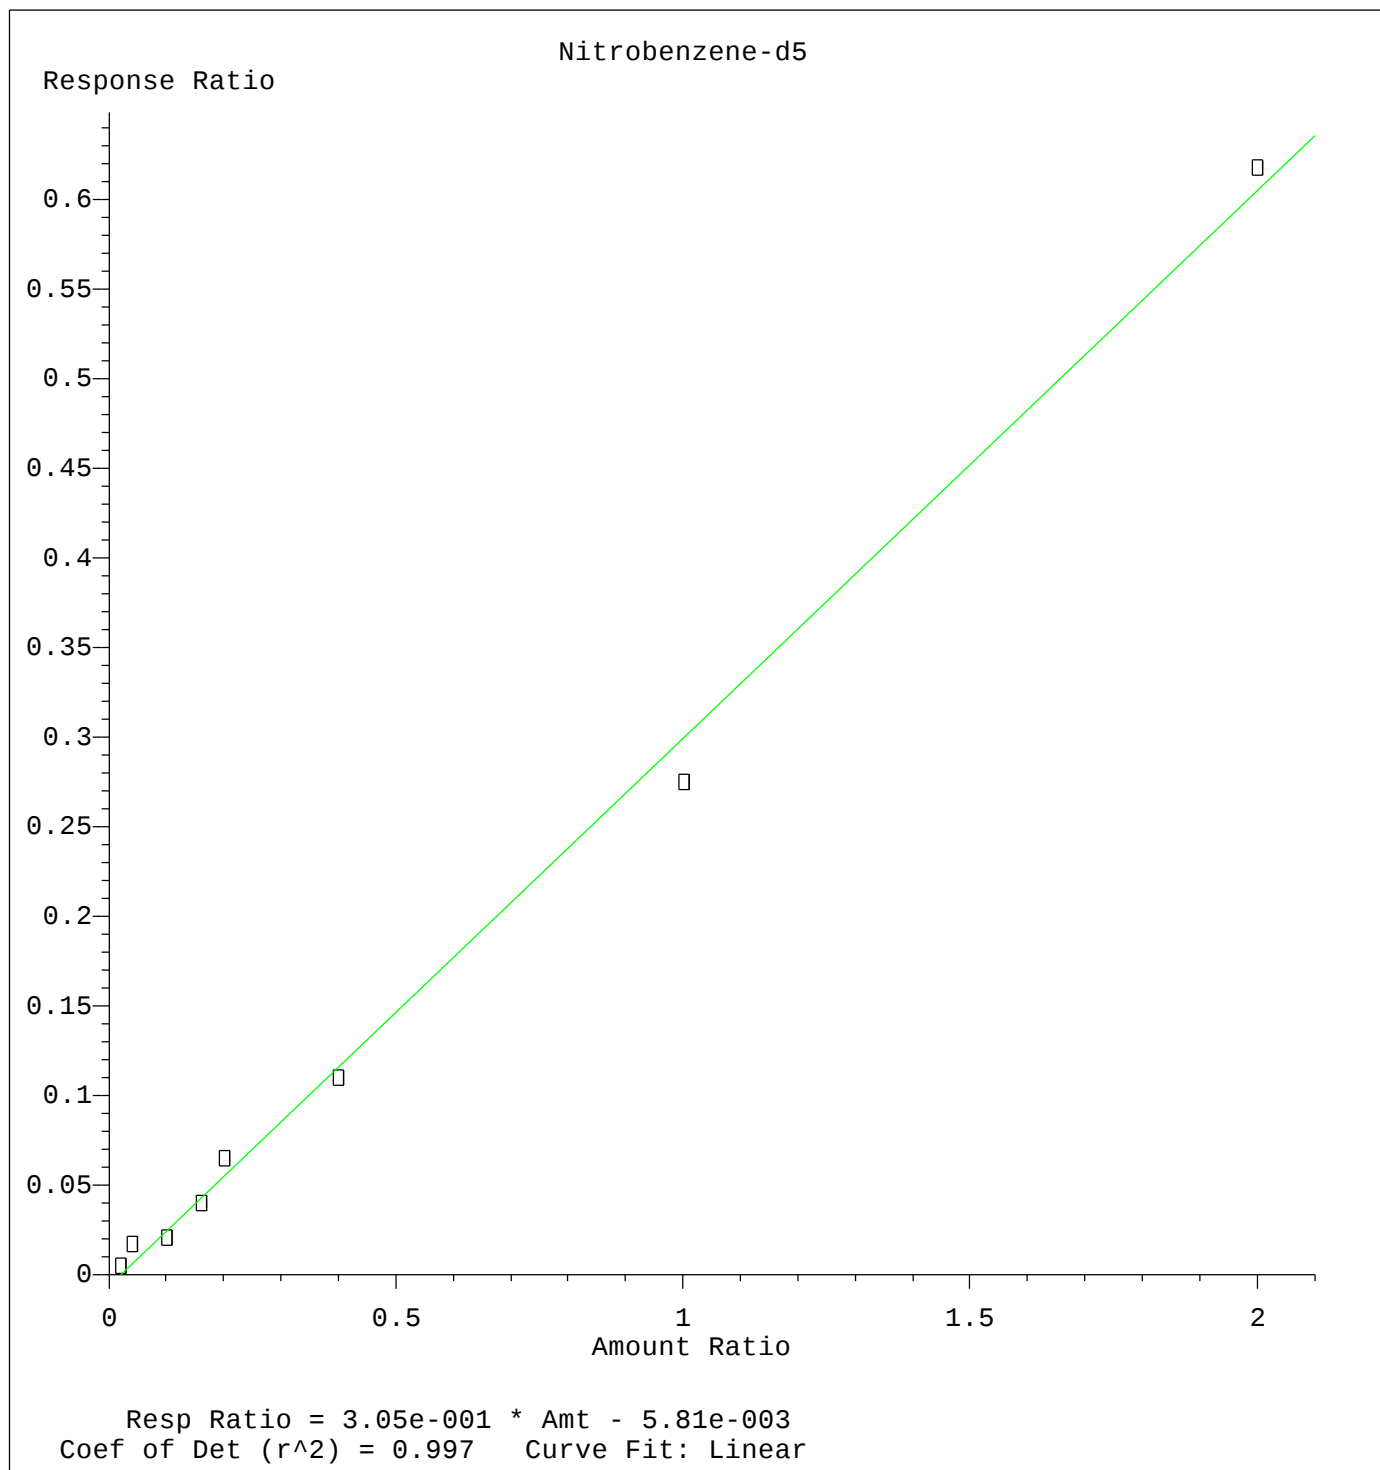

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Calibration Table Last Updated: Tue Feb 24 03:39:32 2015

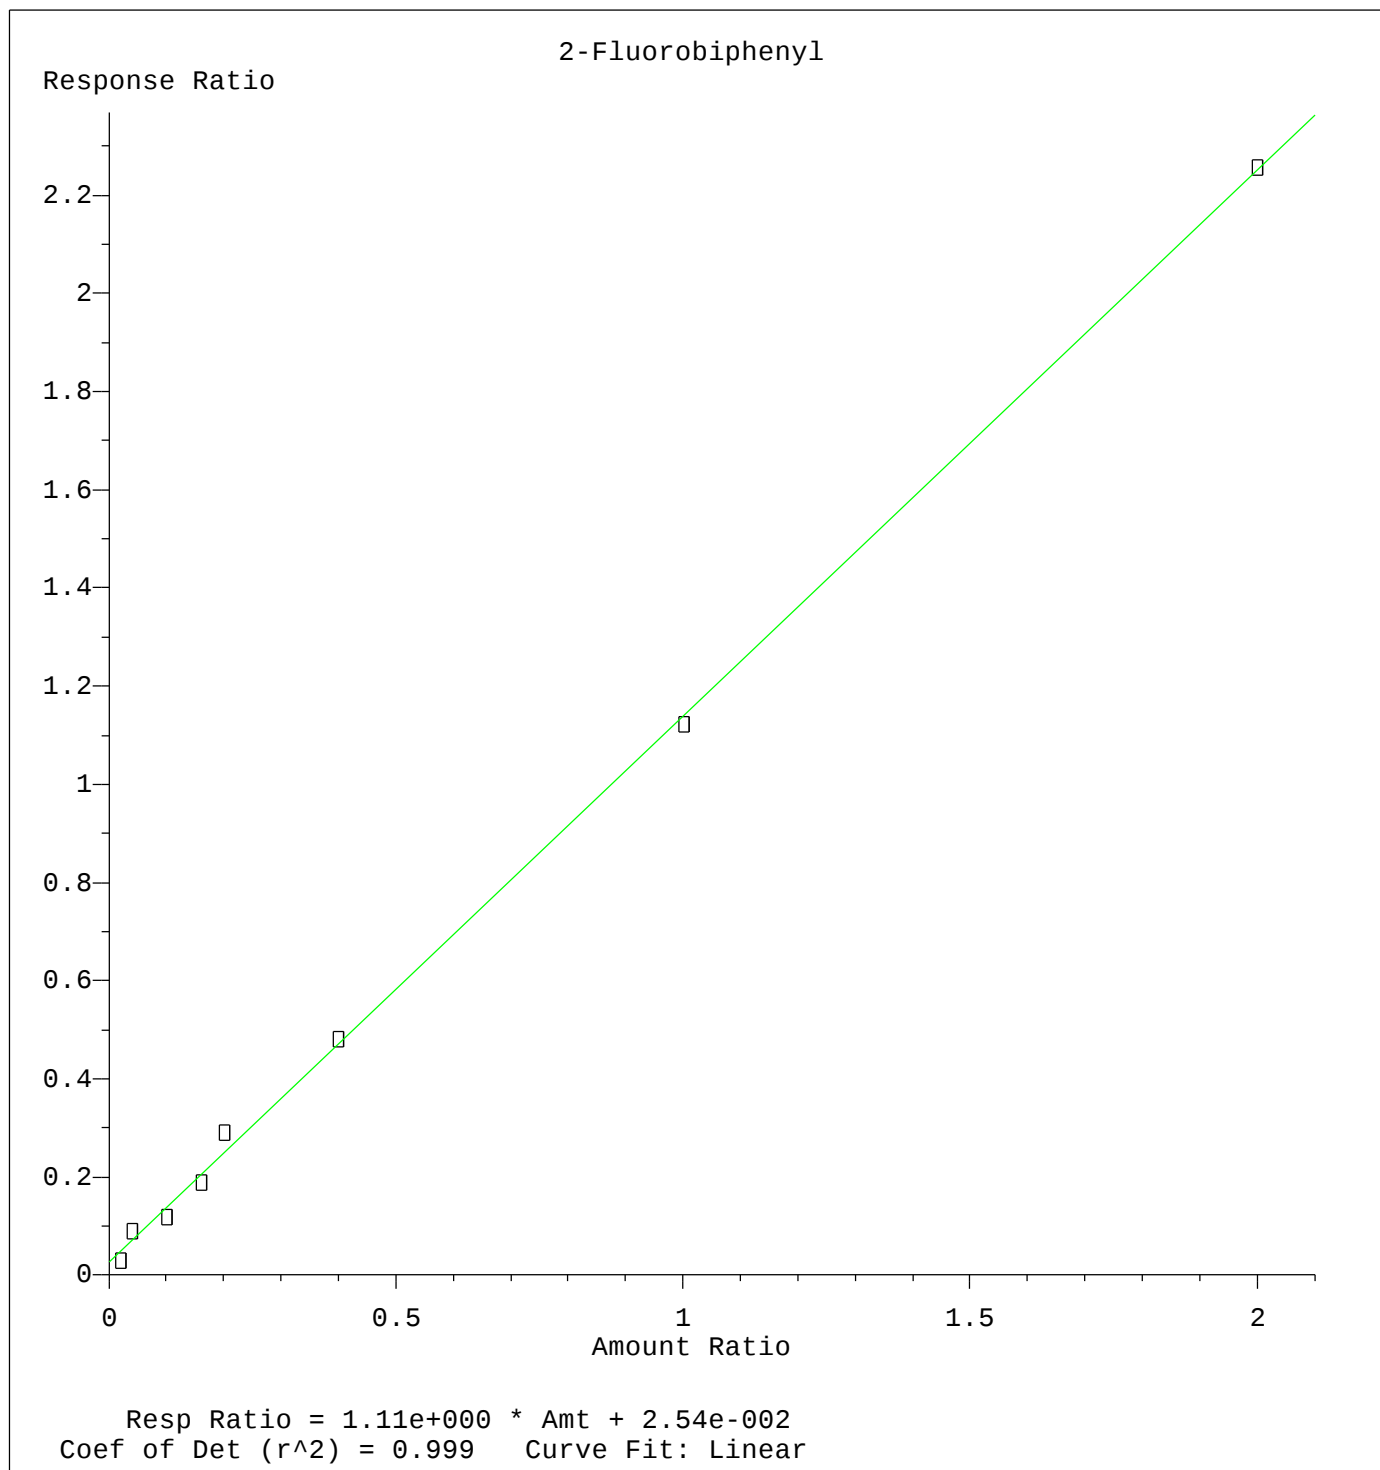


Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Calibration Table Last Updated: Tue Feb 24 03:39:53 2015

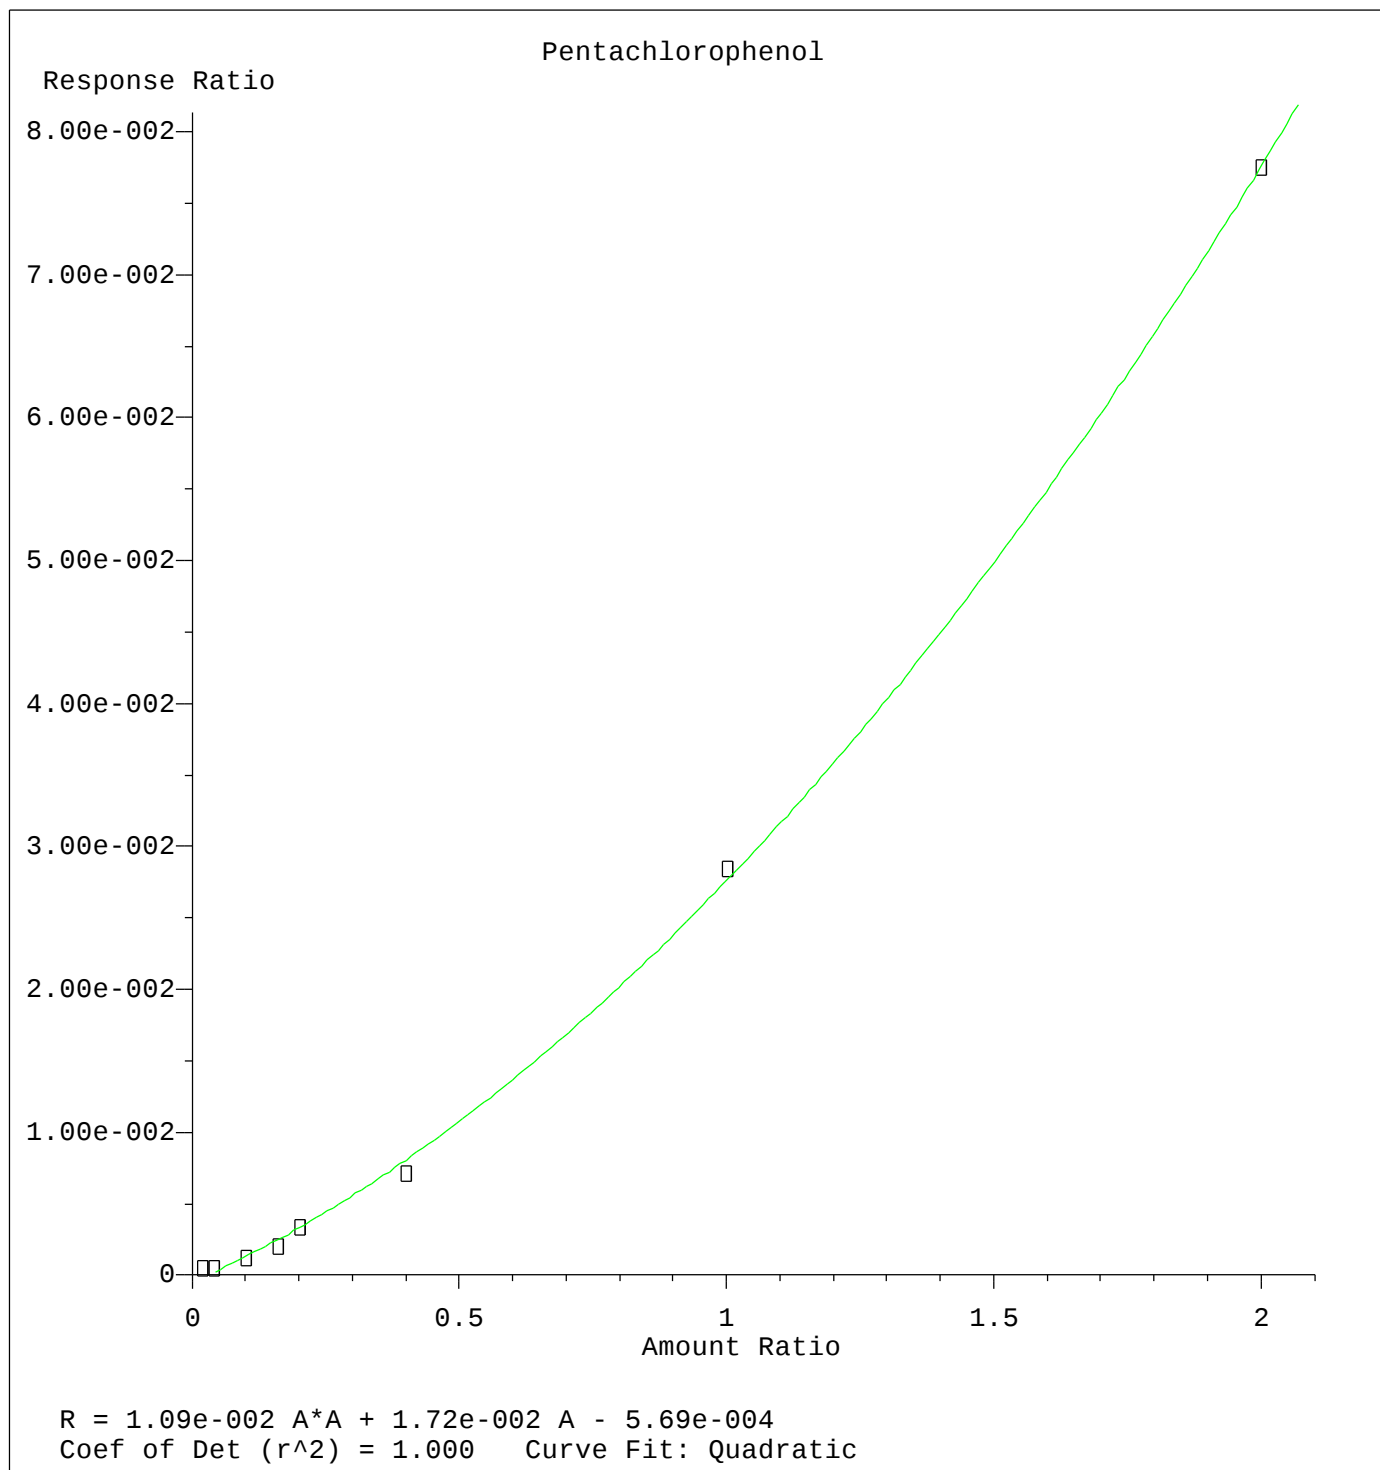

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Calibration Table Last Updated: Tue Feb 24 03:40:13 2015


Indeno(1,2,3-cd)pyrene

Response Ratio

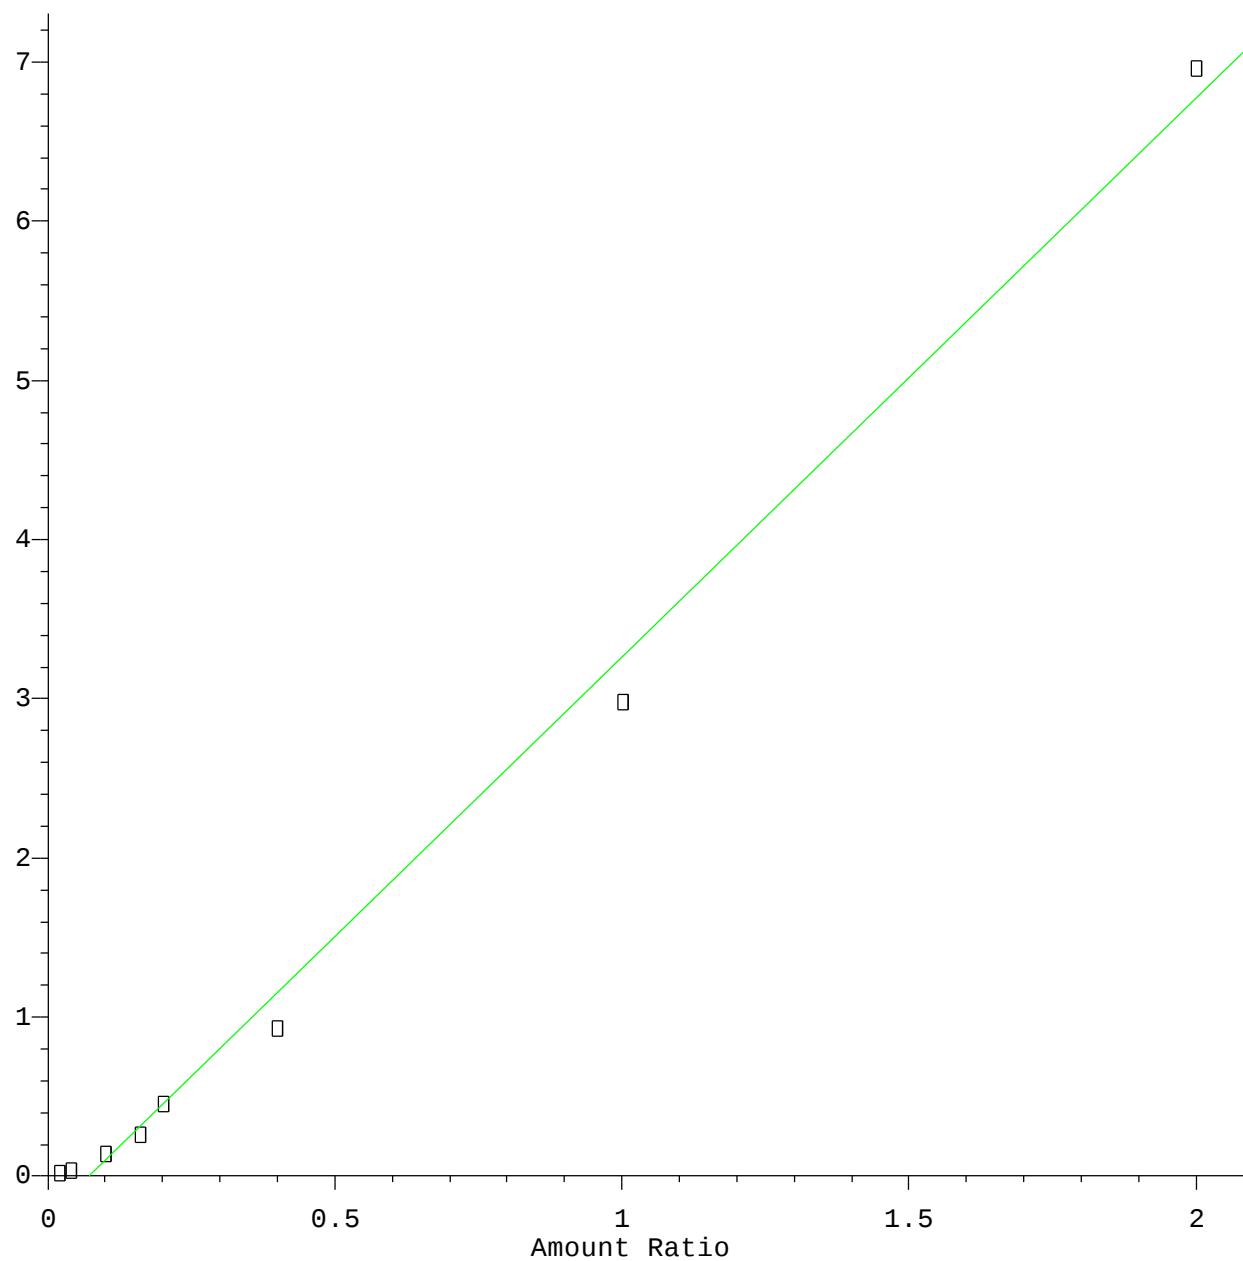


Resp Ratio = 3.51×10^0 * Amt - 2.51×10^{-1}
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Calibration Table Last Updated: Tue Feb 24 03:40:39 2015

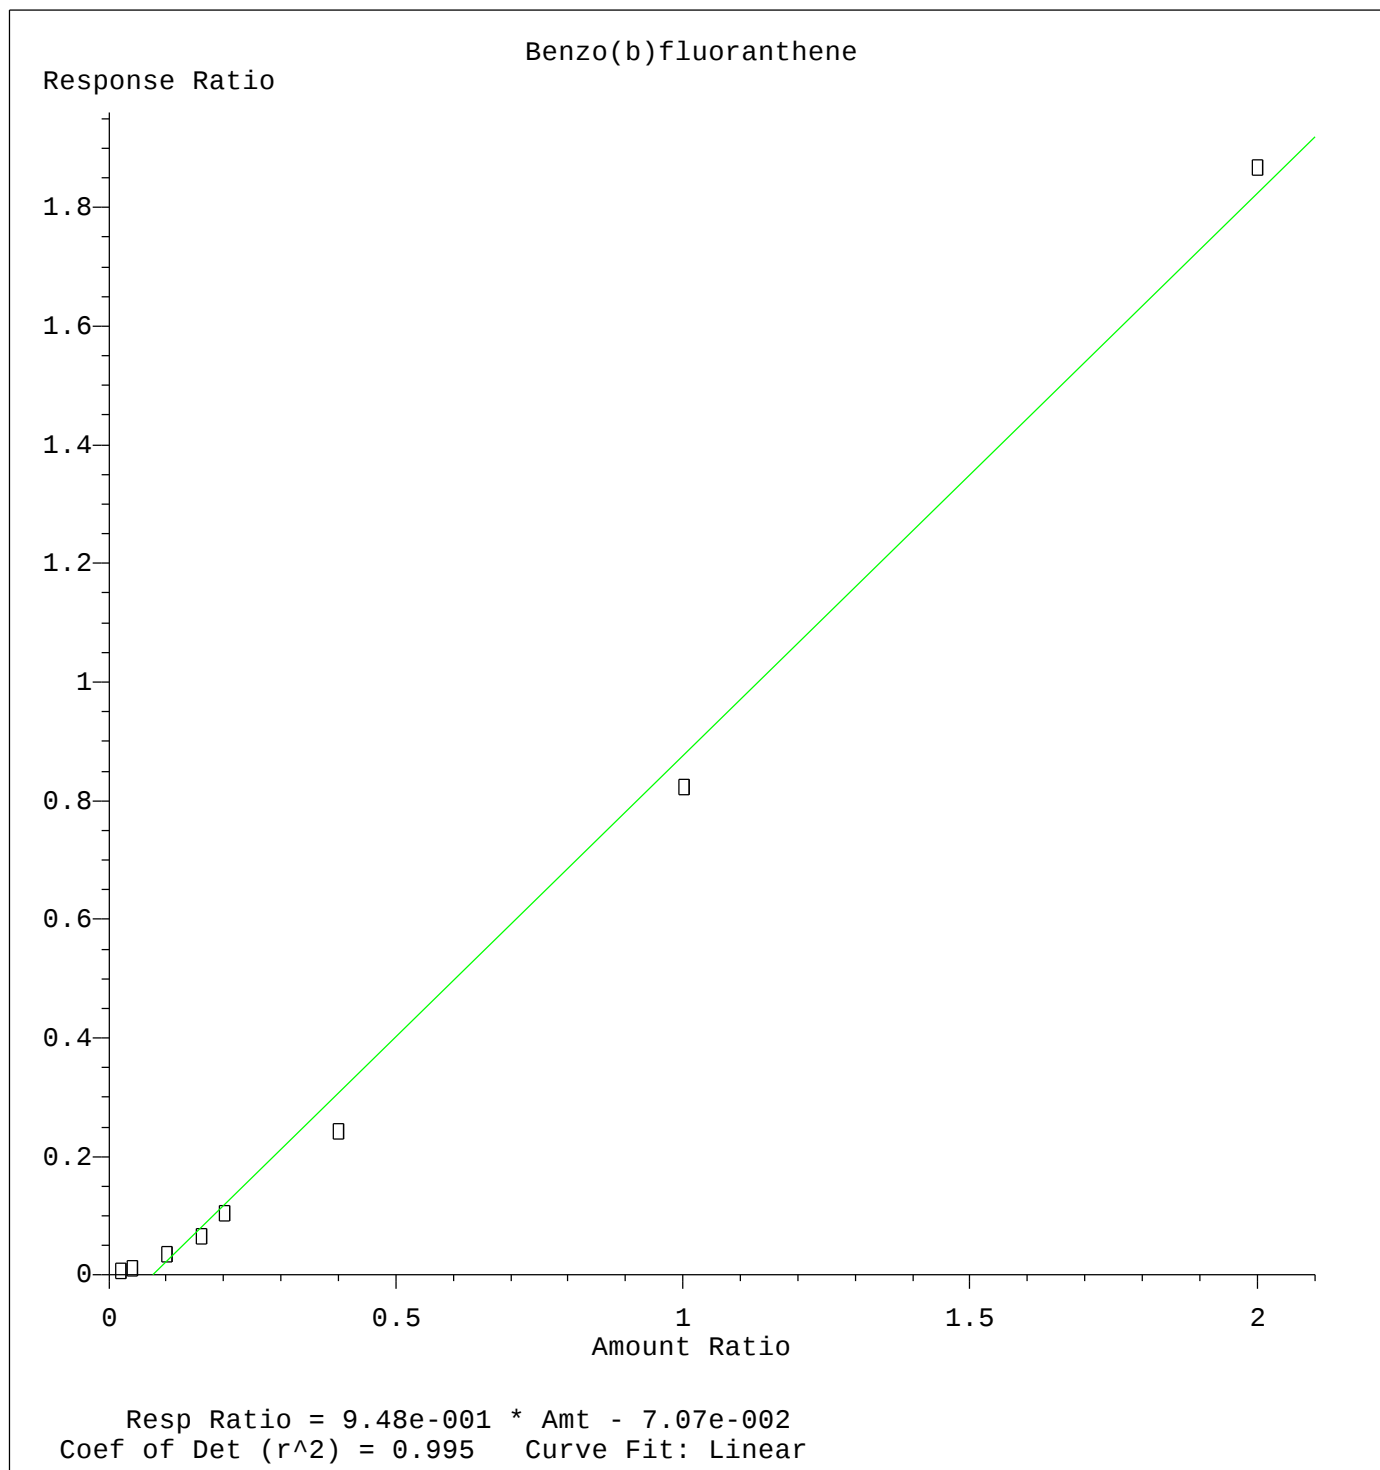

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Calibration Table Last Updated: Tue Feb 24 03:44:54 2015

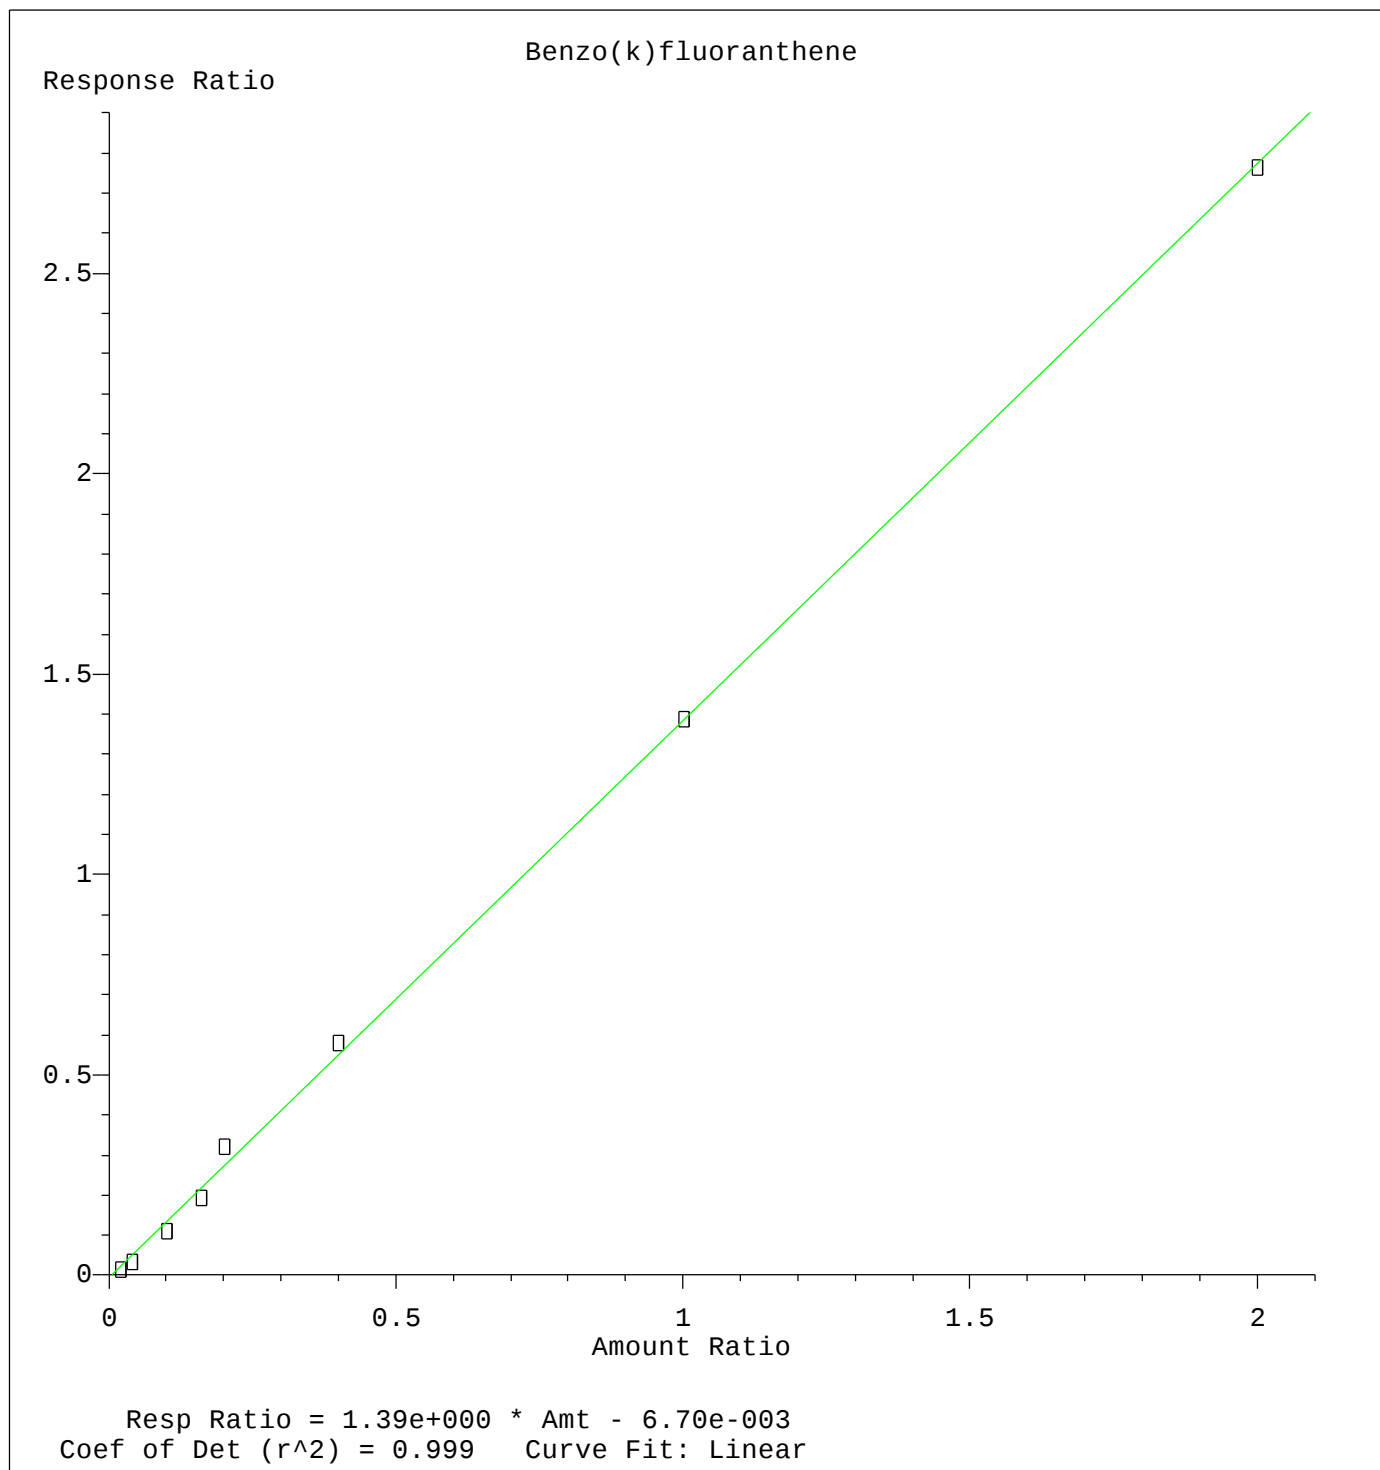


Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Calibration Table Last Updated: Tue Feb 24 03:45:14 2015

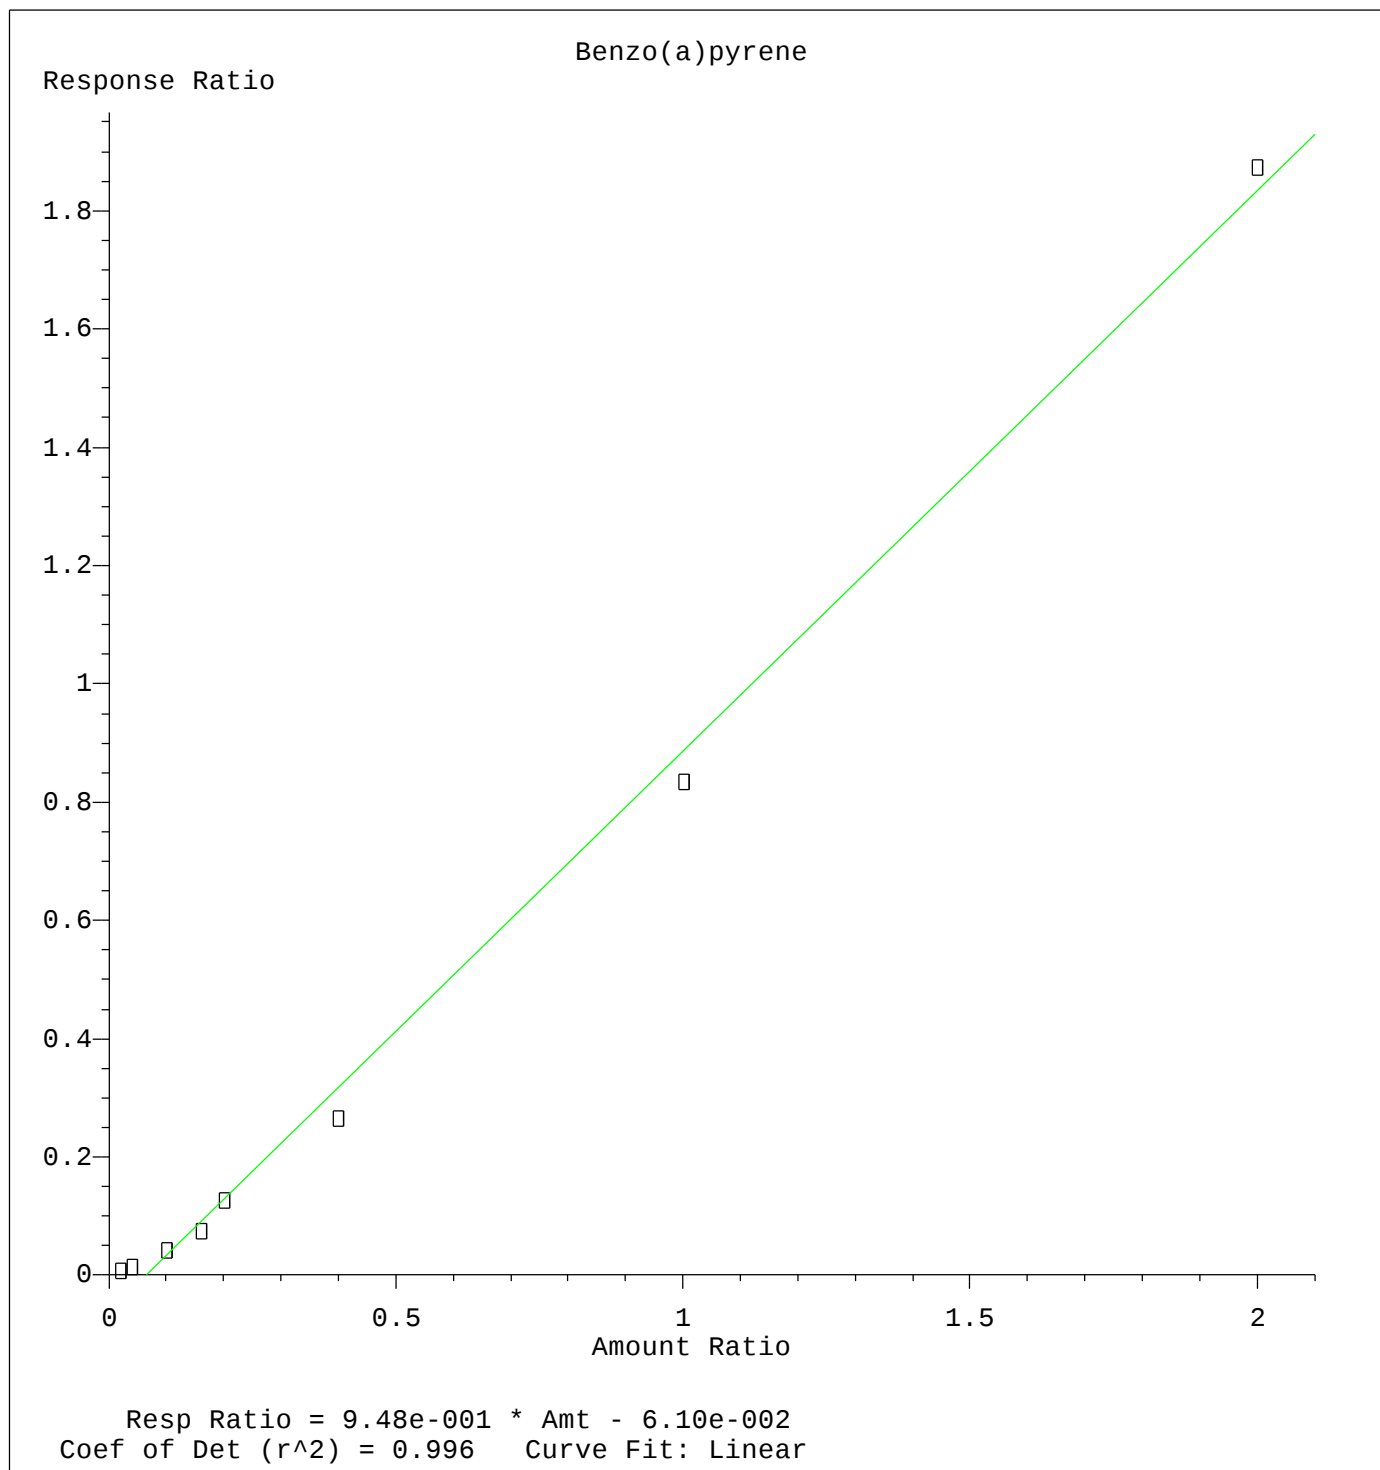

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Calibration Table Last Updated: Tue Feb 24 03:45:29 2015


Dibenzo(a,h)anthracene

Response Ratio

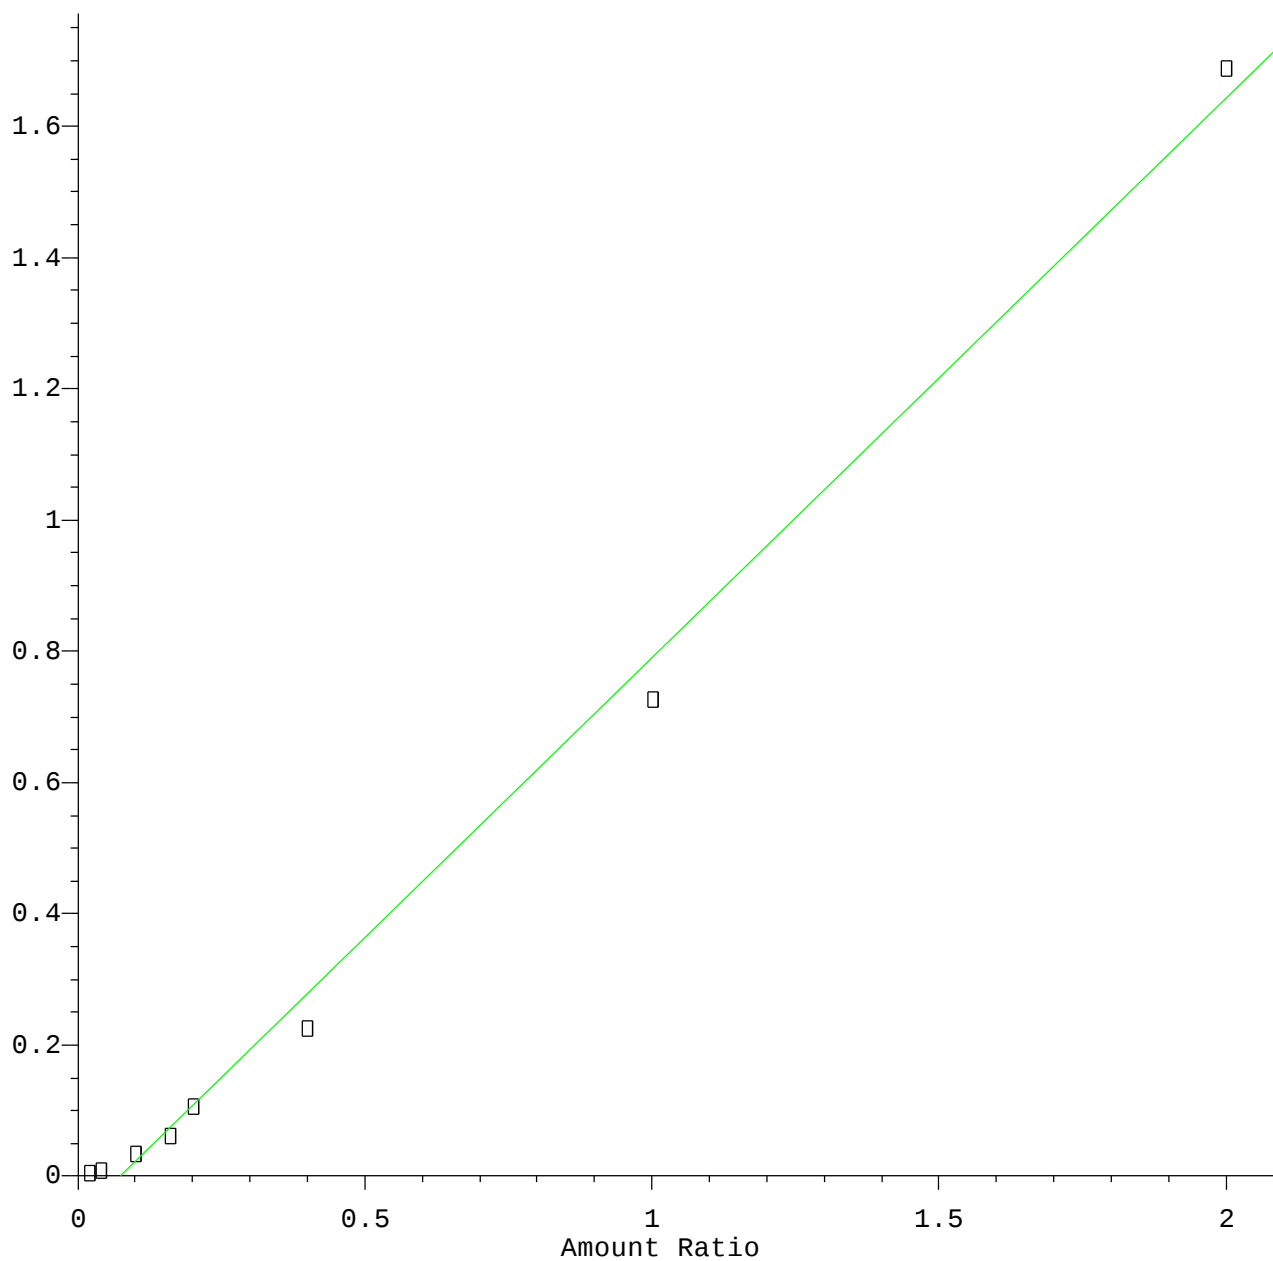

Resp Ratio = $8.53 \times 10^{-1} \times \text{Amt} - 6.19 \times 10^{-2}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Calibration Table Last Updated: Tue Feb 24 03:45:43 2015

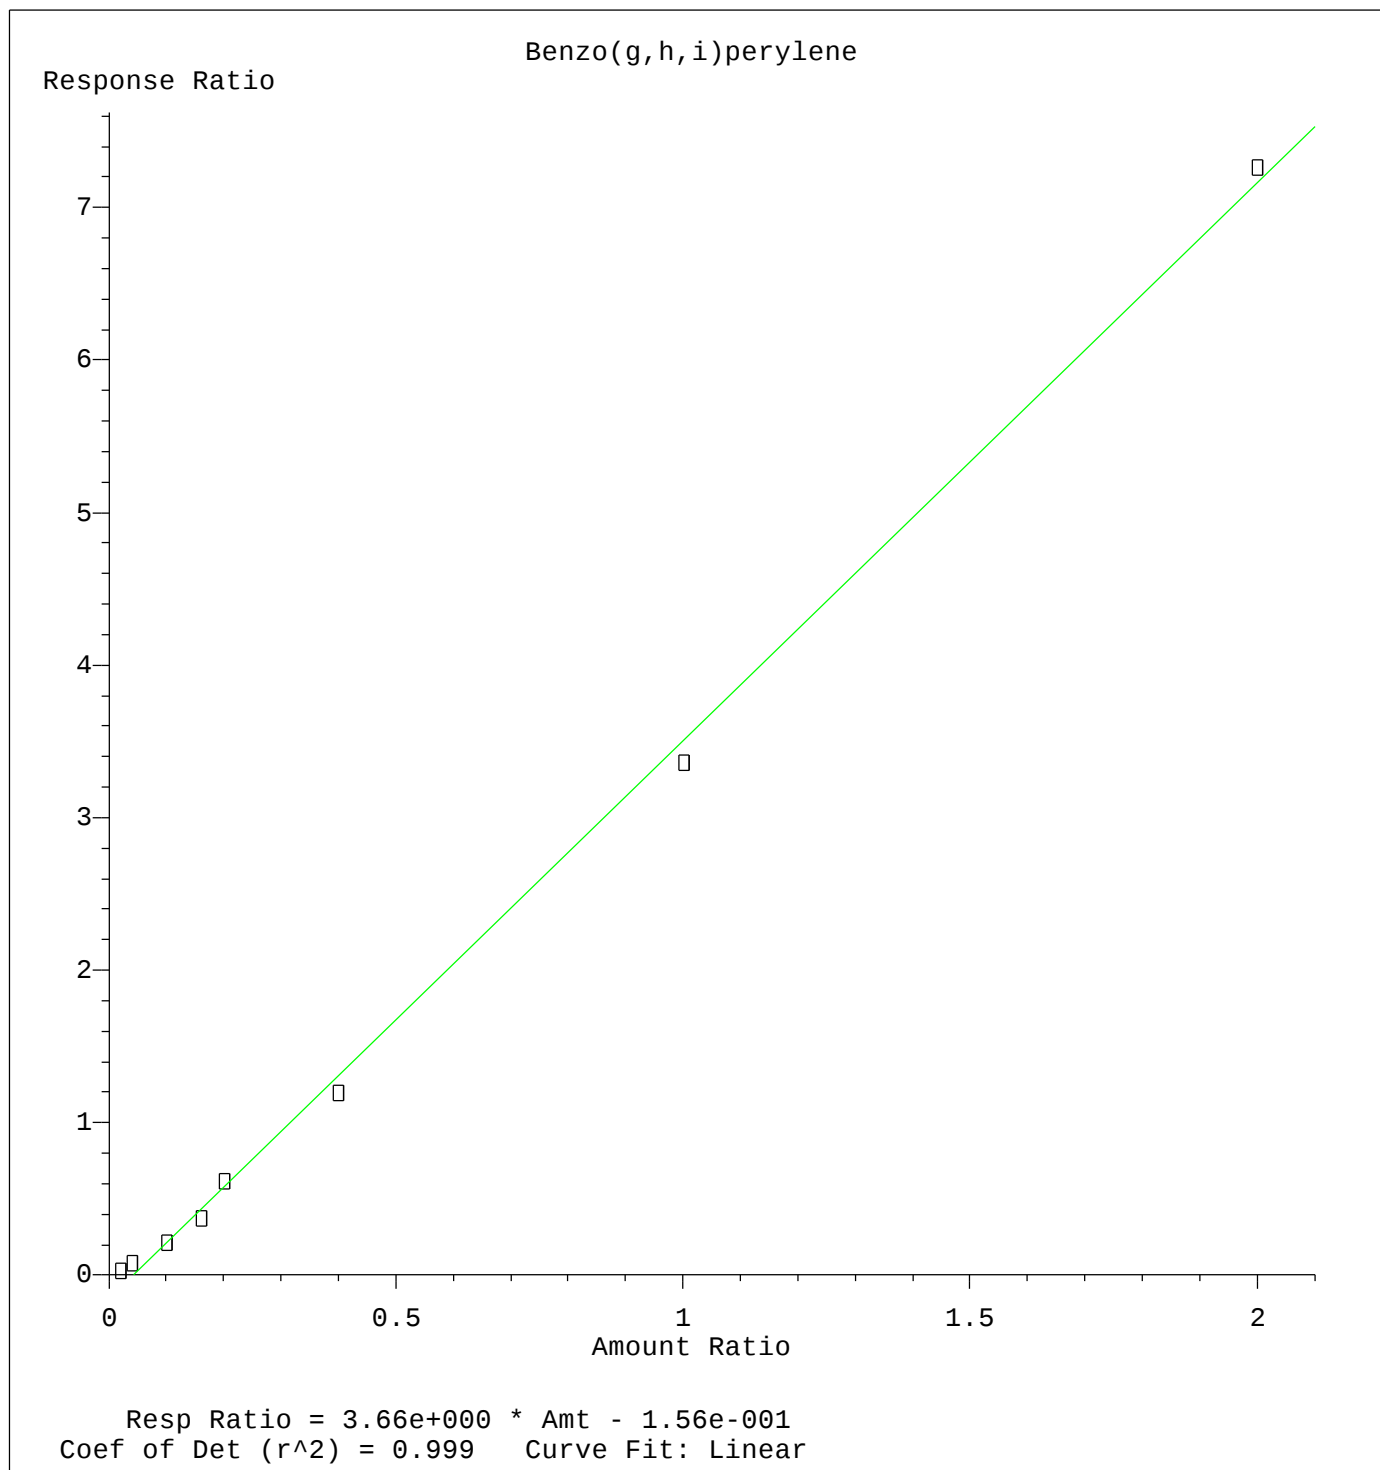

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Calibration Table Last Updated: Tue Feb 24 03:46:00 2015