


Data Path : Z:\HPCHEM1\BNA E\DATA\BE022315\
Data File : BE089647.D
Acq On : 23 Feb 2015 17:37
Operator : TP/JJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 24 03:46:57 2015

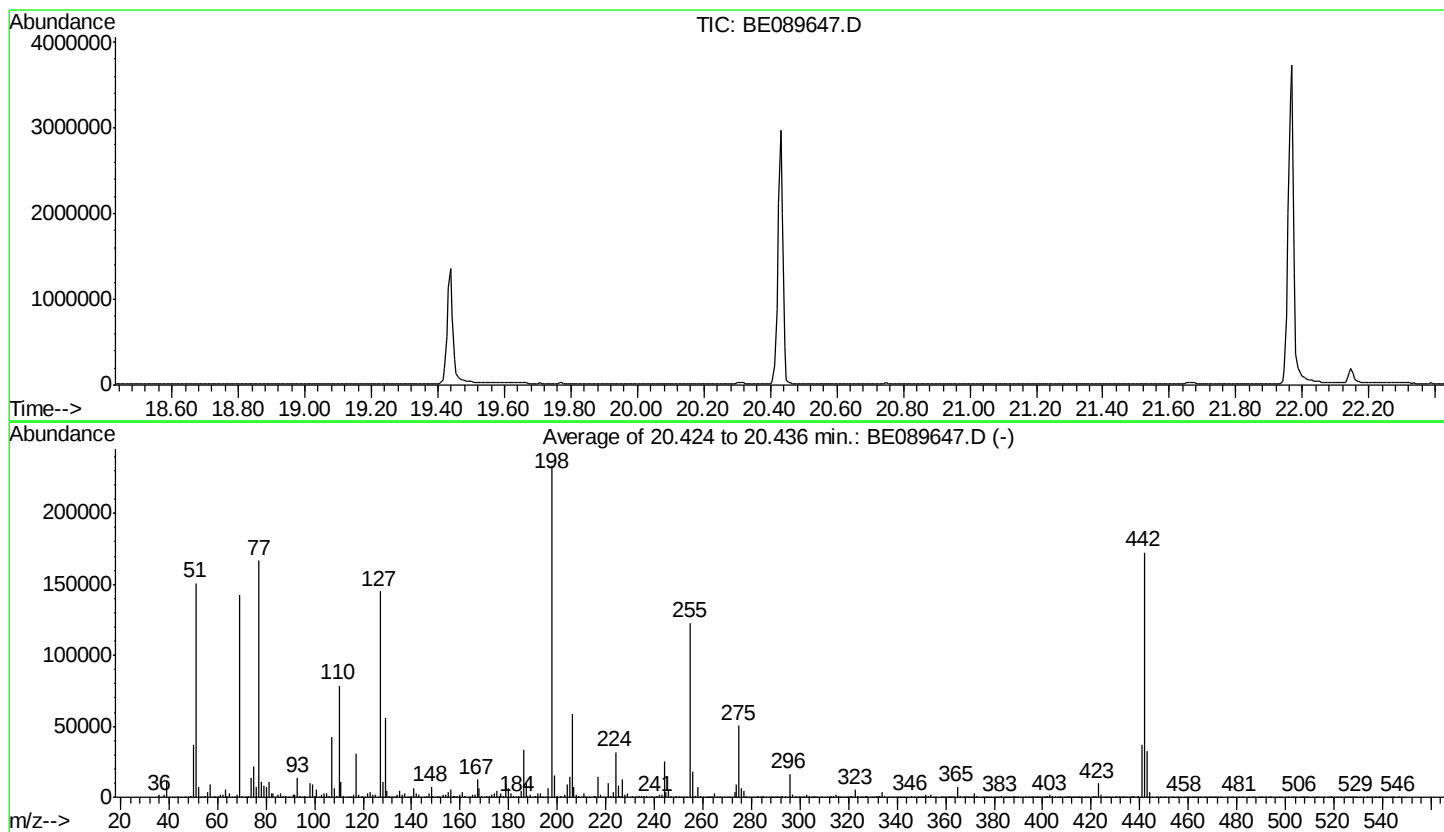

AutoFind: Scans 3240, 3241, 3242; Background Corrected with Scan 3232

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.5	150694	PASS
68	69	0.00	2	1.4	1931	PASS
69	198	0.00	100	61.0	142597	PASS
70	69	0.00	2	0.5	645	PASS
127	198	10	80	62.0	144965	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	233666	PASS
199	198	5	9	6.7	15633	PASS
275	198	10	60	21.6	50517	PASS
365	198	1	100	3.2	7550	PASS
441	442	0.01	24	21.7	37419	PASS
442	198	50	100	73.9	172602	PASS
443	442	15	24	19.0	32731	PASS