

Data Path : Z:\HPCHEM1\BNA E\Data\BE022318\
 Data File : BE095675.D
 Acq On : 23 Feb 2018 10:17
 Operator : SJ/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 23 11:06:40 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE022318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 23 10:57:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.434	152	1172	0.40	ng	0.00
7) Naphthalene-d8	11.260	136	4687	0.40	ng	-0.02
13) Acenaphthene-d10	15.000	164	2644	0.40	ng	0.00
19) Phenanthrene-d10	17.714	188	5930	0.40	ng	0.01
27) Chrysene-d12	21.792	240	6247	0.40	ng	0.00
34) Perylene-d12	24.421	264	5506	0.40	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.916	112	2413	0.68	ng	0.00
5) Phenol-d6	7.552	99	3325	0.68	ng	0.00
8) Nitrobenzene-d5	9.598	82	3492	0.70	ng	-0.02
11) 2-Methylnaphthalene-d10	12.805	152	6066	0.78	ng	0.00
14) 2,4,6-Tribromophenol	16.472	330	751	0.62	ng	0.00
15) 2-Fluorobiphenyl	13.637	172	9263	0.81	ng	0.00
25) Fluoranthene-d10	19.687	212	59792	0.77	ng	0.00
29) Terphenyl-d14	20.252	244	9802	0.74	ng	0.00


Target Compounds						Qvalue
2) 1,4-Dioxane	3.650	88	1411	0.73	ng	# 90
3) n-Nitrosodimethylamine	3.989	42	1823	0.75	ng	# 85
6) bis(2-Chloroethyl)ether	7.829	93	3380	0.75	ng	96
9) Naphthalene	11.310	128	41708	0.77	ng	99
10) Hexachlorobutadiene	11.572	225	2522	0.86	ng	96
12) 2-Methylnaphthalene	12.877	142	7222	0.78	ng	98
16) Acenaphthylene	14.733	152	11520	0.76	ng	99
17) Acenaphthene	15.059	154	7400	0.79	ng	97
18) Fluorene	16.024	166	9097	0.77	ng	# 78
20) 4-Bromophenyl-phenylether	16.891	248	2866	0.80	ng	# 71
21) Hexachlorobenzene	17.026	284	2906	0.79	ng	# 82
22) Pentachlorophenol	17.355	266	694	0.68	ng	# 75
23) Phenanthrene	17.744	178	14401	0.79	ng	98
24) Anthracene	17.833	178	13077	0.77	ng	95
26) Fluoranthene	19.716	202	17840	0.78	ng	# 97
28) Pyrene	20.065	202	20694	0.79	ng	98
30) Benzo(a)anthracene	21.777	228	16089	0.77	ng	97
31) Chrysene	21.839	228	15797	0.77	ng	99
32) Bis(2-ethylhexyl)phtha...	21.652	149	26438	0.55	ng	100
33) Indeno(1,2,3-cd)pyrene	27.229	276	15473	0.78	ng	# 94
35) Benzo(b)fluoranthene	23.605	252	15181	0.81	ng	# 88
36) Benzo(k)fluoranthene	23.660	252	15434	0.80	ng	95
37) Benzo(a)pyrene	24.302	252	13884	0.79	ng	# 93
38) Dibenzo(a,h)anthracene	27.247	278	12535	0.82	ng	# 96
39) Benzo(g,h,i)perylene	28.099	276	13102	0.80	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\Data\BE022318\
Data File : BE095675.D
Acq On : 23 Feb 2018 10:17
Operator : SJ/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 23 11:06:40 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE022318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 10:57:33 2018
Response via : Initial Calibration

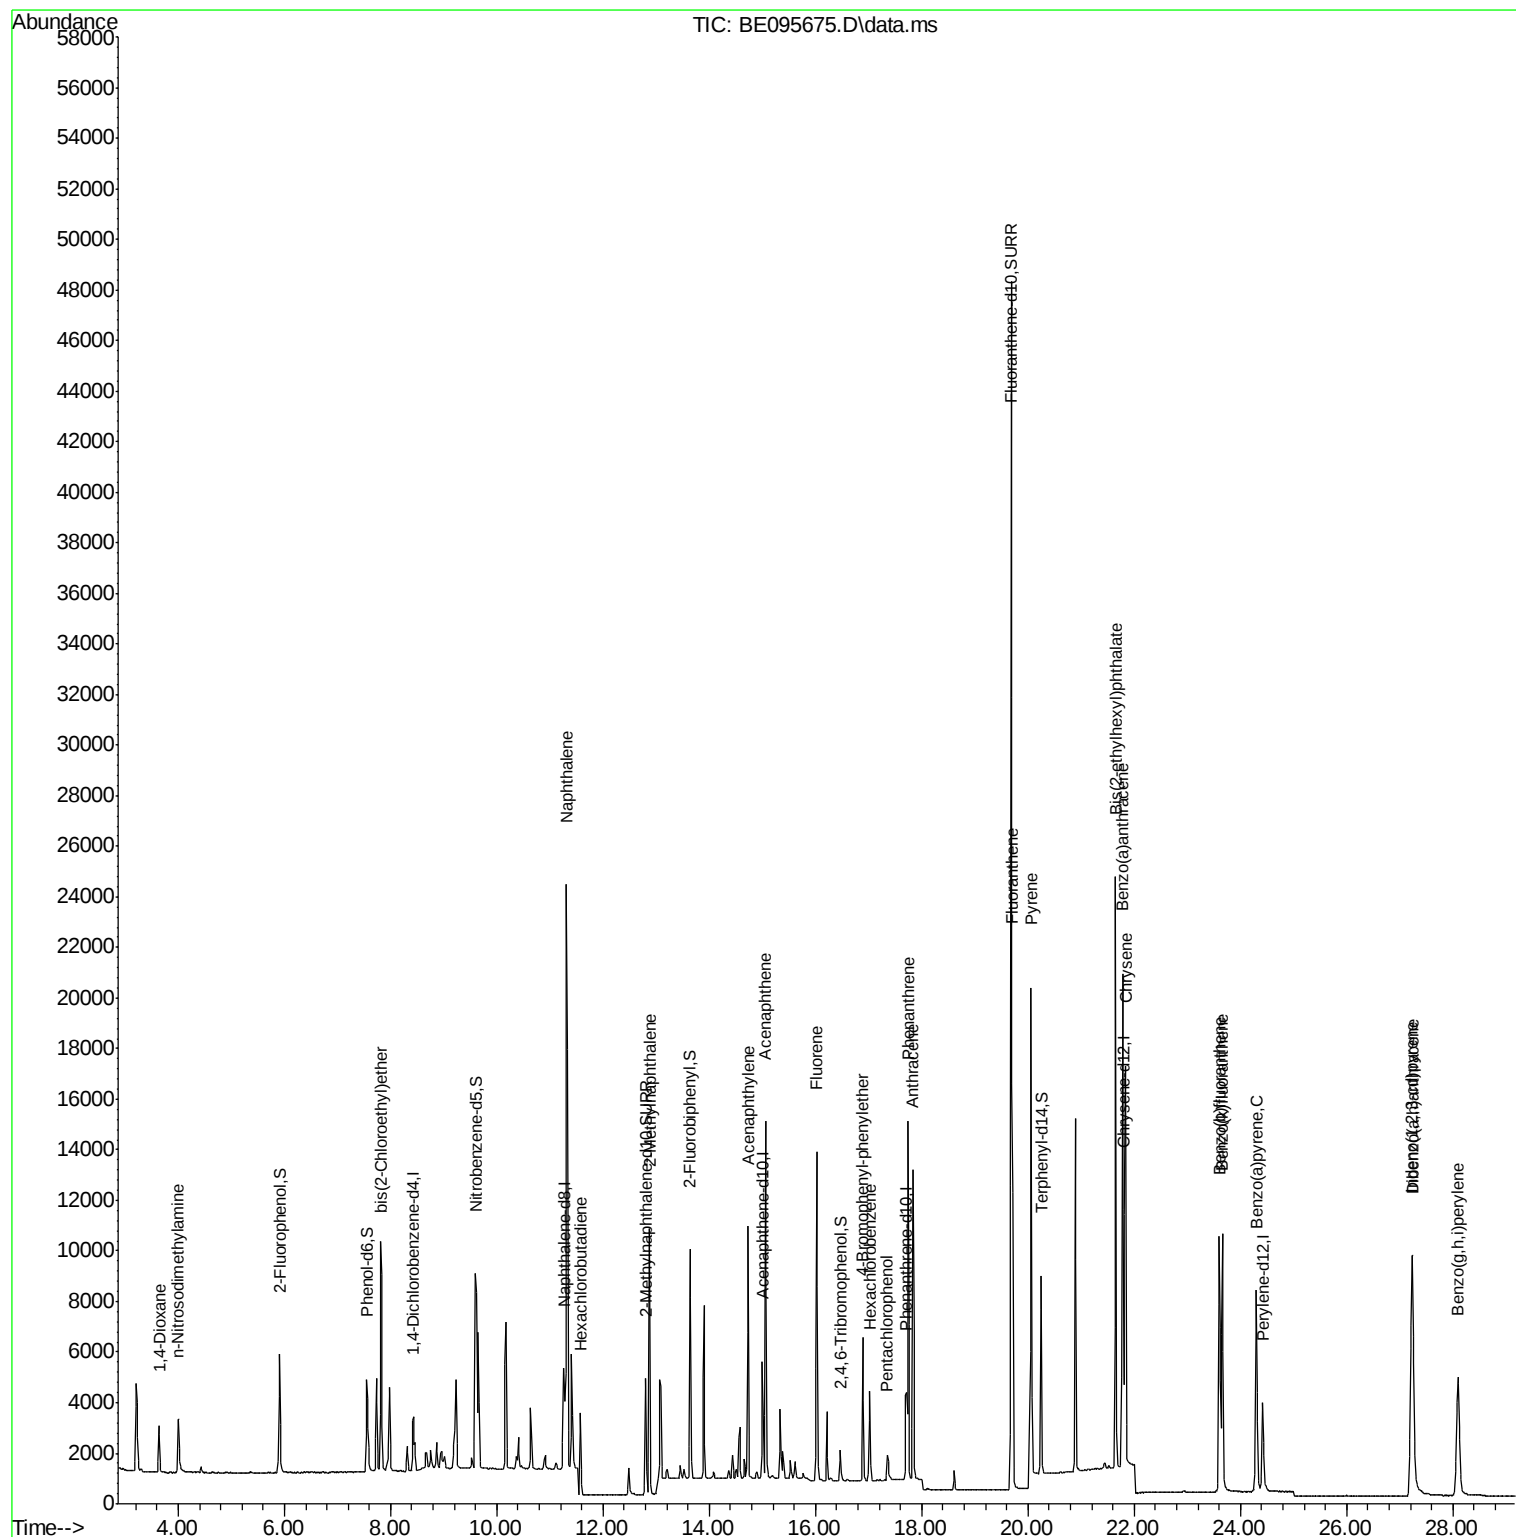



#1

1,4-Dichlorobenzene-d4

Concen: 0.40 ng

RT: 8.434 min Scan# 44

Delta R.T. -0.000 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:152 Resp: 1172

Ion Ratio Lower Upper

152 100

150 136.0 117.2 175.8

115 64.1 57.0 85.6

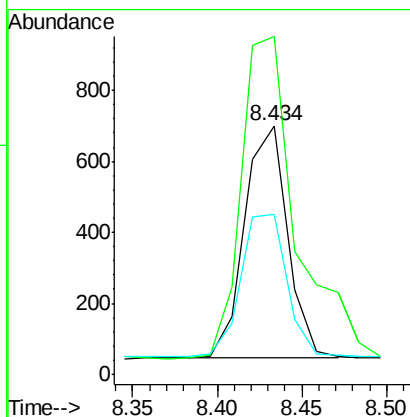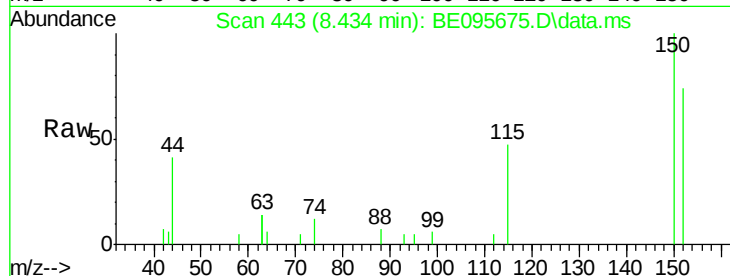

#2

1,4-Dioxane

Concen: 0.73 ng

RT: 3.650 min Scan# 63

Delta R.T. -0.000 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion: 88 Resp: 1411


Ion Ratio Lower Upper

88 100

58 80.9 63.2 94.8

43 36.1 41.2 61.8#

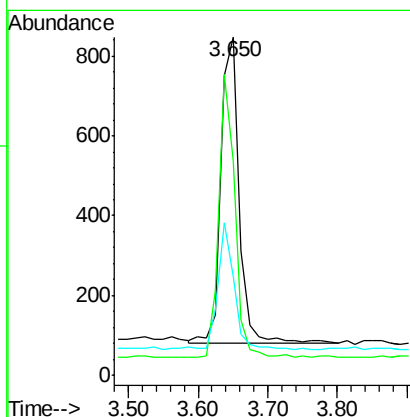

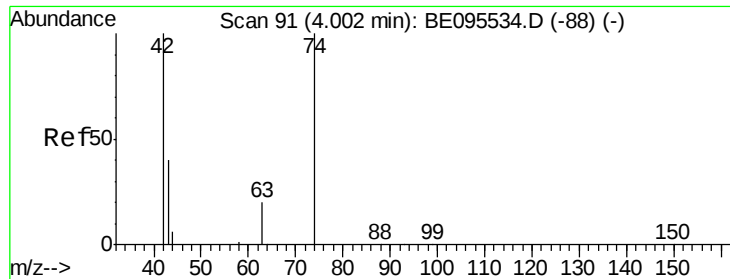

#3

n-Nitrosodimethylamine

Concen: 0.75 ng

RT: 3.989 min Scan# 90

Delta R.T. -0.013 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17





Instrument :

BNA_E

ClientSampleId :

Tot Ion: 42 Resp: 1823

Ion	Ratio	Lower	Upper
42	100		
74	103.6	96.0	144.0
44	8.1	12.0	18.0#

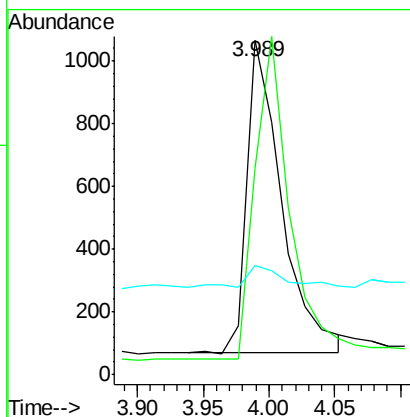

#4

2-Fluorophenol

Concen: 0.68 ng

RT: 5.916 min Scan# 243




Delta R.T. -0.000 min




Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Tgt Ion: 112 Resp: 2413

Ion	Ratio	Lower	Upper
112	100		
64	72.2	60.1	90.1
63	156.4	116.8	175.2

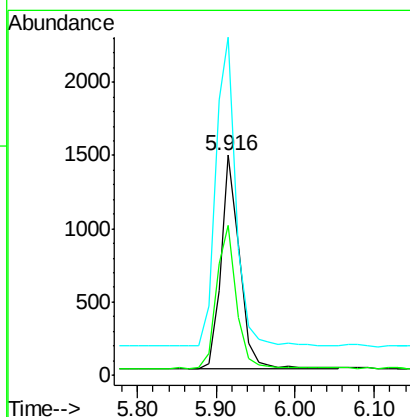

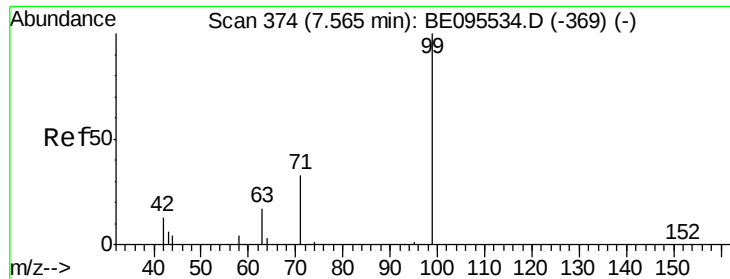

#5

Phenol-d6

Concen: 0.68 ng

RT: 7.552 min Scan# 37

Delta R.T. -0.000 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion: 99 Resp: 3325

Ion Ratio Lower Upper

99 100

42 25.9 20.2 30.2

71 41.1 28.4 42.6

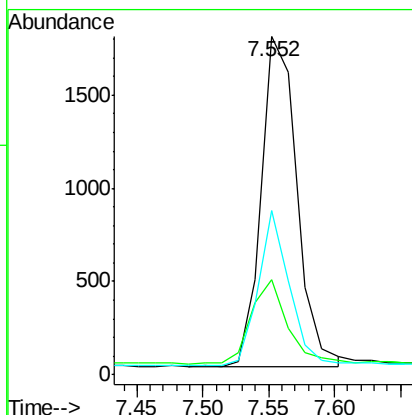

#6

bis(2-Chloroethyl)ether

Concen: 0.75 ng

RT: 7.829 min Scan# 395

Delta R.T. -0.000 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17


Tgt Ion: 93 Resp: 3380


Ion Ratio Lower Upper

93 100

63 334.8 275.3 412.9

95 31.9 25.2 37.8

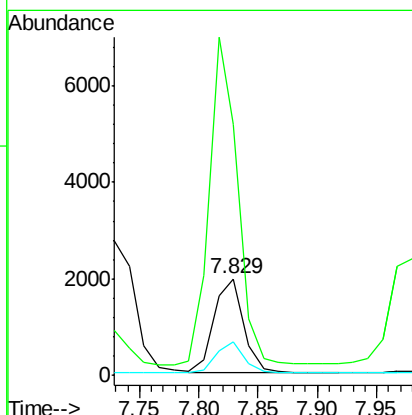

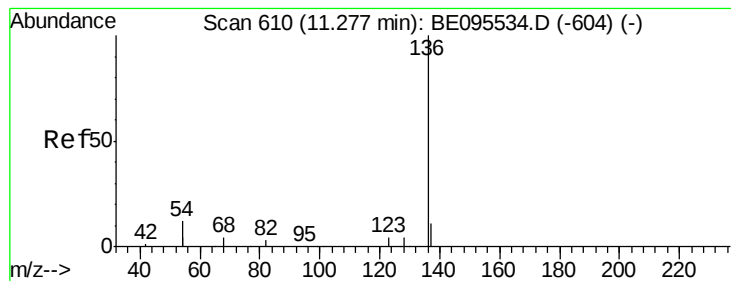

#7

Naphthalene-d8

Concen: 0.40 ng

RT: 11.260 min Scan# 60

Delta R.T. -0.016 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :

Tot Ion:136 Resp: 4687





Ion Ratio Lower Upper

136 100

137 12.2 9.5 14.3

54 62.9 29.1 43.7#

68 11.6 6.2 9.2#

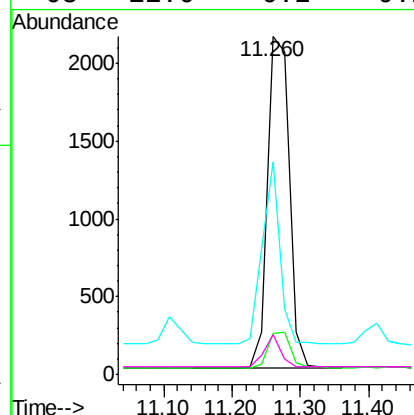

#8

Nitrobenzene-d5

Concen: 0.70 ng

RT: 9.598 min Scan# 510

Delta R.T. -0.016 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion: 82 Resp: 3492


Ion Ratio Lower Upper

82 100

128 85.7 150.0 225.0#

54 285.3 154.2 231.4#

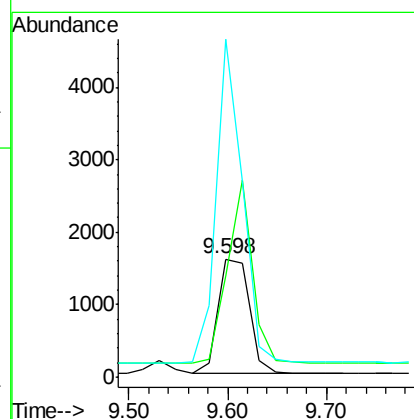

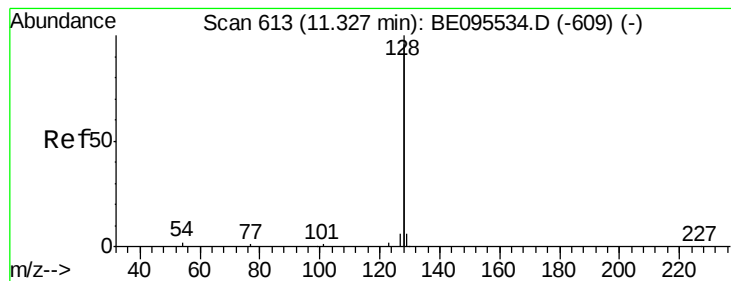

#9

Naphthalene

Concen: 0.77 ng

RT: 11.310 min Scan# 61

Delta R.T. 0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:128 Resp: 41708

Ion Ratio Lower Upper

128 100

129 3.0 2.6 3.8

127 3.7 2.8 4.2

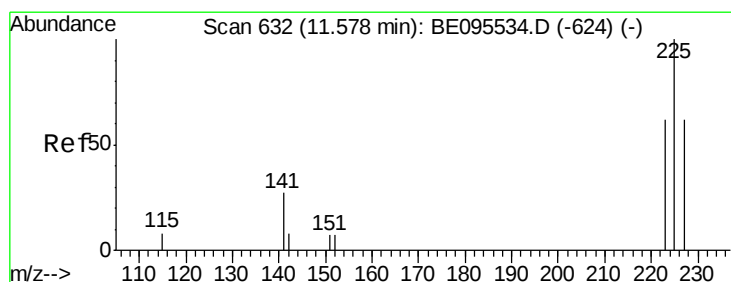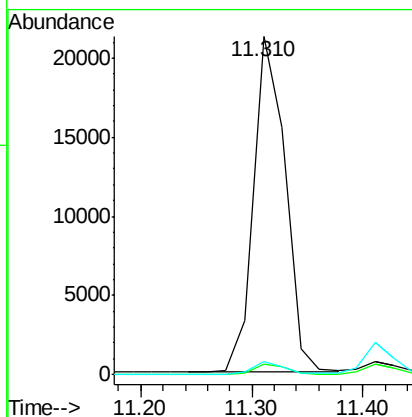

#10

Hexachlorobutadiene

Concen: 0.86 ng

RT: 11.572 min Scan# 631

Delta R.T. 0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:225 Resp: 2522


Ion Ratio Lower Upper

225 100

223 61.1 53.0 79.6

227 62.8 51.4 77.2

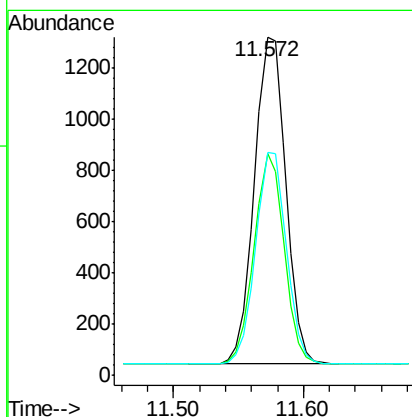

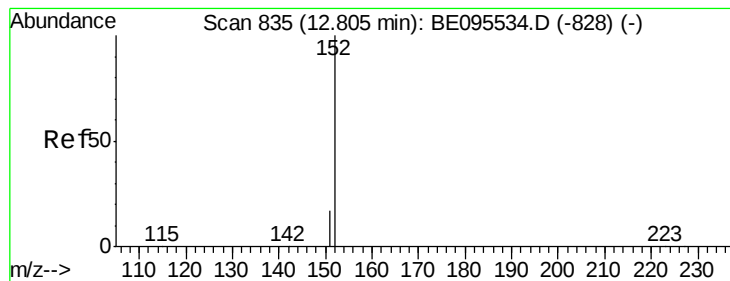

#11

2-Methylnaphthalene-d10

Concen: 0.78 ng

RT: 12.805 min Scan# 83

Delta R.T. 0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E





ClientSampleId :

Tot Ion:152 Resp: 6066

Ion Ratio Lower Upper

152 100

151 19.7 15.4 23.0

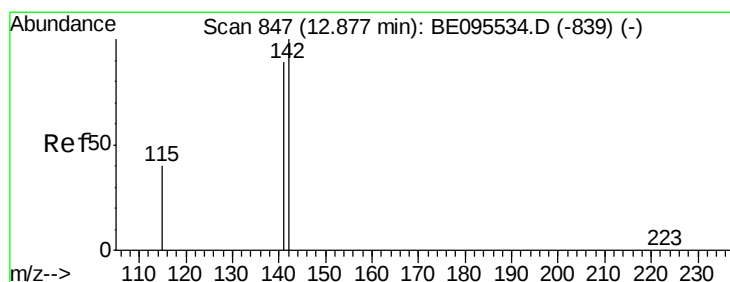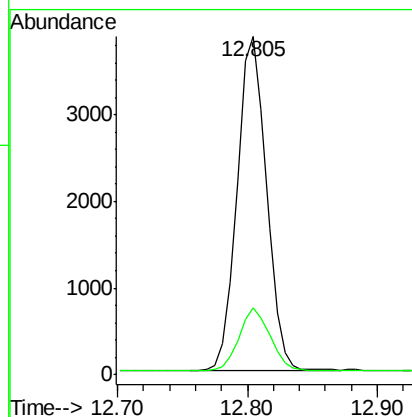

#12

2-Methylnaphthalene

Concen: 0.78 ng

RT: 12.877 min Scan# 847

Delta R.T. 0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:142 Resp: 7222


Ion Ratio Lower Upper

142 100

141 89.7 70.4 105.6

115 41.4 31.7 47.5

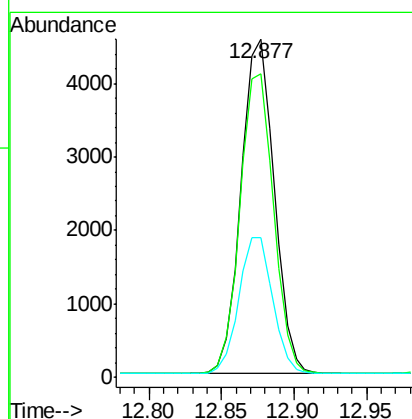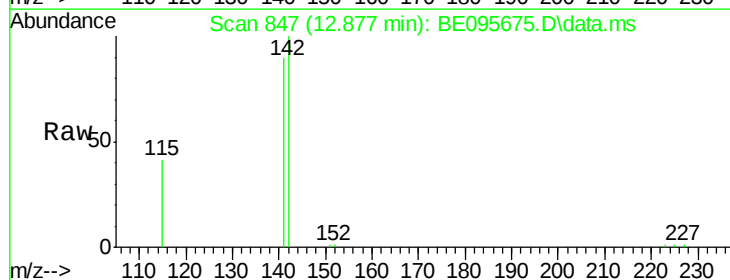



#13

Acenaphthene-d10

Concen: 0.40 ng

RT: 15.000 min Scan# 1000

Delta R.T. -0.002 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:164 Resp: 2644

Ion Ratio Lower Upper

164 100

162 109.2 83.1 124.7

160 49.9 37.1 55.7

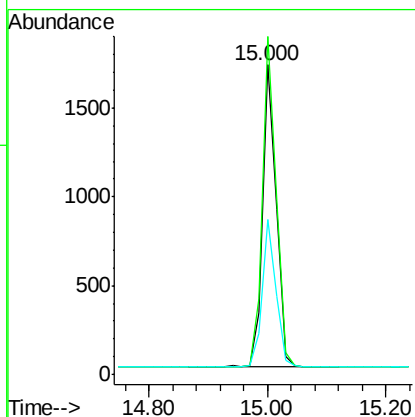

#14

2,4,6-Tribromophenol

Concen: 0.62 ng

RT: 16.472 min Scan# 1096

Delta R.T. -0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:330 Resp: 751


Ion Ratio Lower Upper

330 100

332 96.9 152.7 229.1#

141 45.0 33.7 50.5

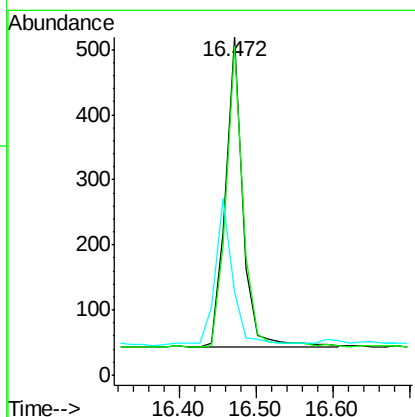

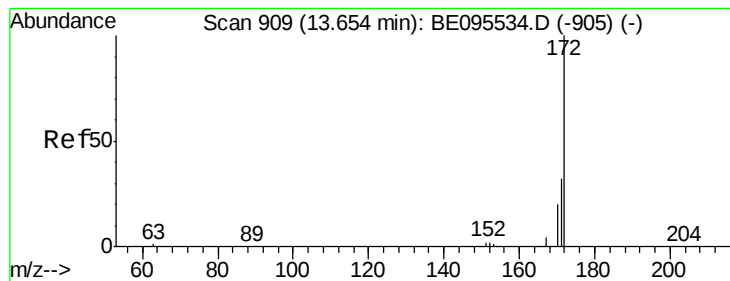

#15

2-Fluorobiphenyl

Concen: 0.81 ng

RT: 13.637 min Scan# 909

Delta R.T. -0.002 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:172 Resp: 9263

Ion Ratio Lower Upper

172 100

171 36.8 29.9 44.9

170 24.7 21.8 32.8

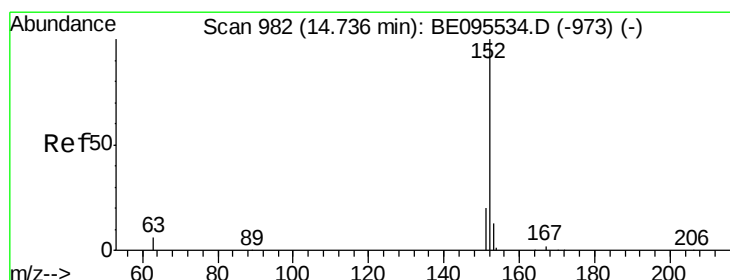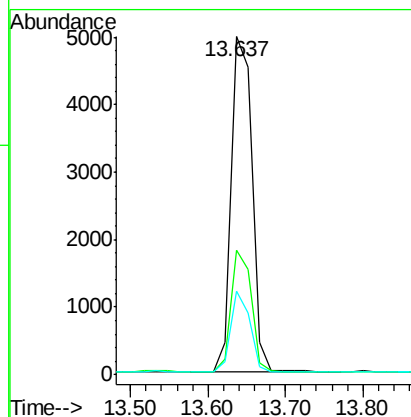

#16

Acenaphthylene

Concen: 0.76 ng

RT: 14.733 min Scan# 982

Delta R.T. -0.002 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:152 Resp: 11520


Ion Ratio Lower Upper

152 100

151 20.0 15.7 23.5

153 13.0 10.5 15.7

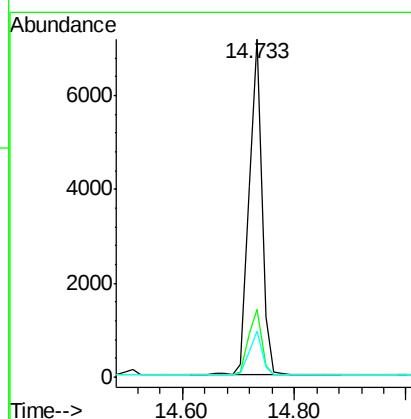



#17

Acenaphthene

Concen: 0.79 ng

RT: 15.059 min Scan# 10

Delta R.T. -0.002 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:154 Resp: 7400

Ion Ratio Lower Upper

154 100

153 113.5 89.2 133.8

152 57.1 42.0 63.0

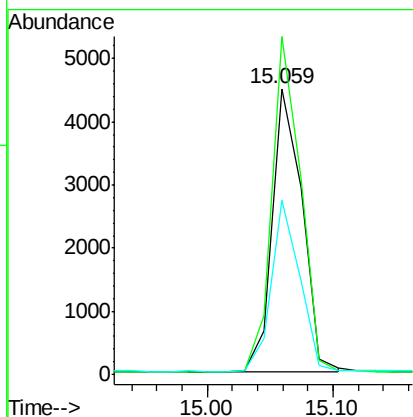

#18

Fluorene

Concen: 0.77 ng

RT: 16.024 min Scan# 1066

Delta R.T. -0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:166 Resp: 9097


Ion Ratio Lower Upper

166 100

165 100.5 77.8 116.6

167 13.2 42.4 63.6#

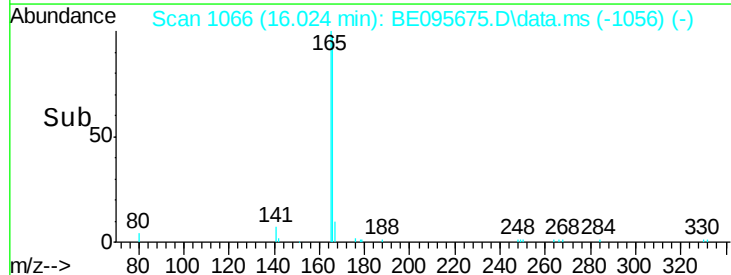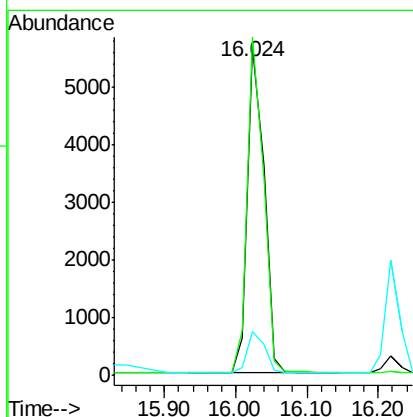

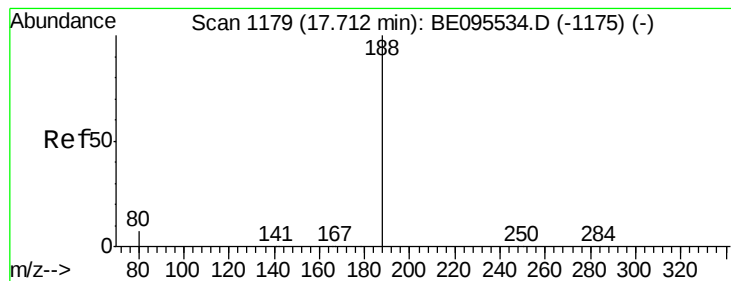

#19

Phenanthrene-d10

Concen: 0.40 ng

RT: 17.714 min Scan# 1179

Delta R.T. 0.014 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:188 Resp: 5930

Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#

80 6.8 3.6 5.4#

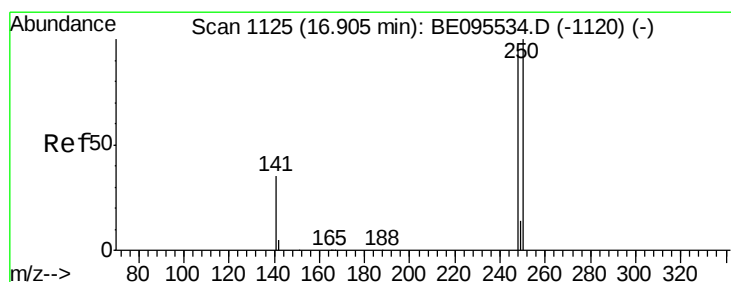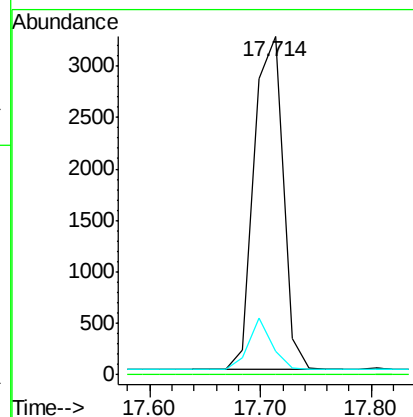

#20

4-Bromophenyl-phenylether

Concen: 0.80 ng

RT: 16.891 min Scan# 1124

Delta R.T. -0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:248 Resp: 2866


Ion Ratio Lower Upper

248 100

250 84.8 62.7 94.1

141 103.4 48.2 72.2#

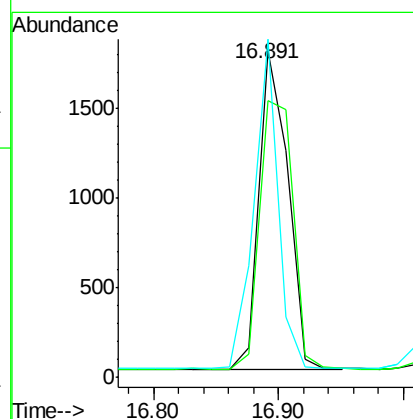



#21

Hexachlorobenzene

Concen: 0.79 ng

RT: 17.026 min Scan# 1133

Delta R.T. -0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:284 Resp: 2906

Ion Ratio Lower Upper

284 100

142 40.6 22.1 33.1#

249 35.1 34.8 52.2

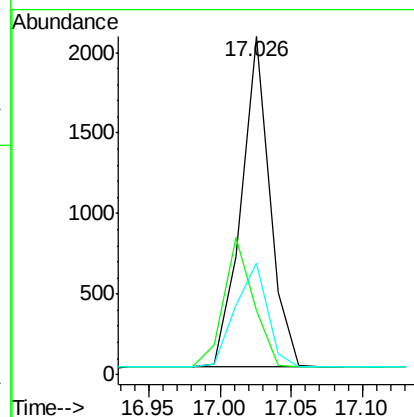

#22

Pentachlorophenol

Concen: 0.68 ng

RT: 17.355 min Scan# 1155

Delta R.T. -0.016 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:266 Resp: 694


Ion Ratio Lower Upper

266 100

264 69.7 72.5 108.7#

268 65.6 73.8 110.6#

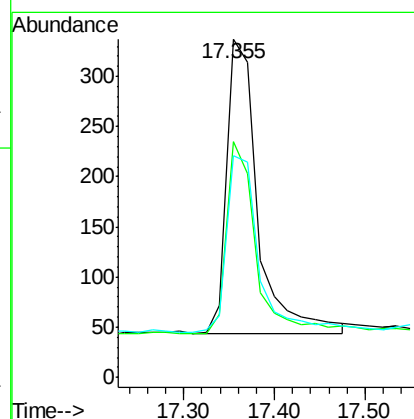



#23

Phenanthrene

Concen: 0.79 ng

RT: 17.744 min Scan# 1181

Delta R.T. -0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:178 Resp: 14401

Ion Ratio Lower Upper

178 100

176 19.8 15.1 22.7

179 15.3 11.8 17.6

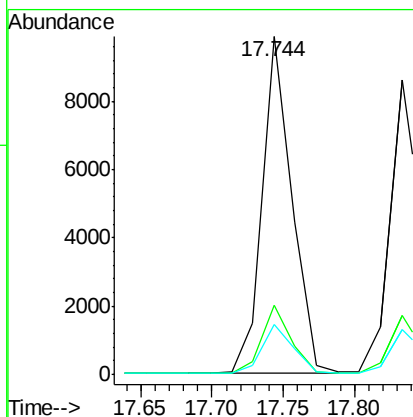

#24

Anthracene

Concen: 0.77 ng

RT: 17.833 min Scan# 1187

Delta R.T. -0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:178 Resp: 13077


Ion Ratio Lower Upper

178 100

176 19.0 12.8 19.2

179 15.1 13.0 19.6



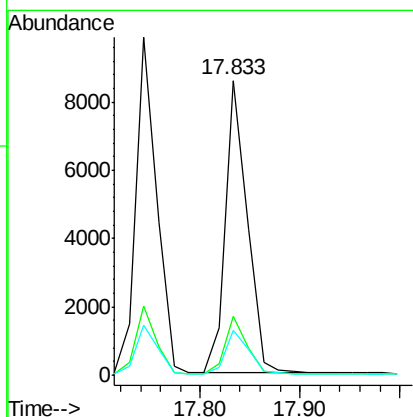





#25
 Fluoranthene-d10
 Concen: 0.77 ng
 RT: 19.687 min Scan# 1422
 Delta R.T. 0.001 min
 Lab File: BE095675.D
 Acq: 23 Feb 2018 10:17




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:212 Resp: 59792
 Ion Ratio Lower Upper
 212 100
 106 2.8 2.8 4.2
 104 1.6 1.6 2.4

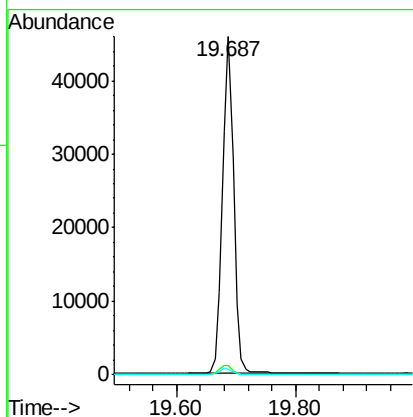

#26
 Fluoranthene
 Concen: 0.78 ng
 RT: 19.716 min Scan# 1426
 Delta R.T. 0.001 min
 Lab File: BE095675.D
 Acq: 23 Feb 2018 10:17

Tgt Ion:202 Resp: 17840
 Ion Ratio Lower Upper
 202 100
 101 9.8 9.8 14.8#
 203 16.9 13.7 20.5

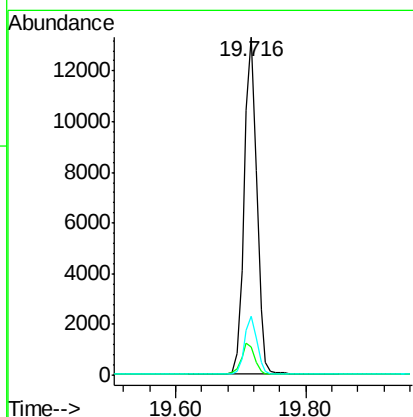



#27

Chrysene-d12

Concen: 0.40 ng

RT: 21.792 min Scan# 15

Delta R.T. -0.000 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:240 Resp: 6247

Ion Ratio Lower Upper

240 100

120 10.2 5.5 8.3#

236 28.8 20.7 31.1

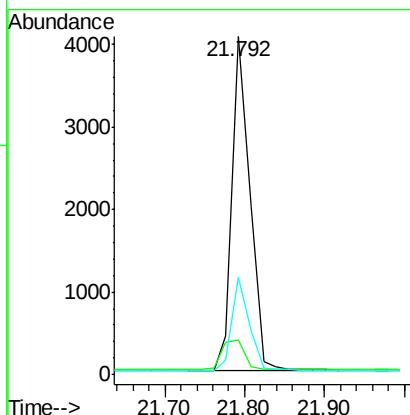

#28

Pyrene

Concen: 0.79 ng

RT: 20.065 min Scan# 1466

Delta R.T. -0.000 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:202 Resp: 20694


Ion Ratio Lower Upper

202 100

200 20.2 16.6 25.0

203 15.9 13.8 20.8

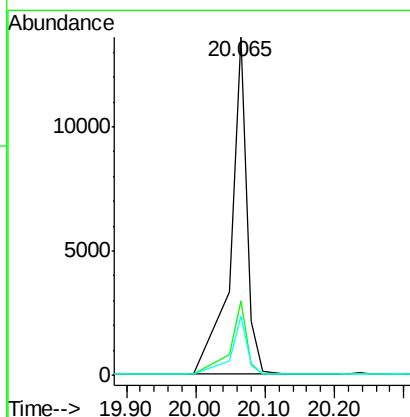



#29

Terphenyl-d14

Concen: 0.74 ng

RT: 20.252 min Scan# 1478

Delta R.T. -0.000 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:244 Resp: 9802

Ion Ratio Lower Upper

244 100

212 6.1 25.4 38.0#

122 2.3 8.1 12.1#

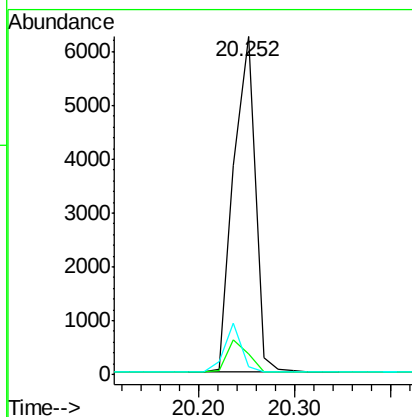

#30

Benzo(a)anthracene

Concen: 0.77 ng

RT: 21.777 min Scan# 1576

Delta R.T. -0.000 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:228 Resp: 16089


Ion Ratio Lower Upper

228 100

226 27.4 24.0 36.0

229 19.7 16.0 24.0

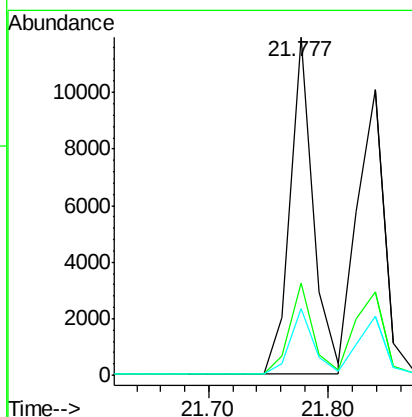



#31

Chrysene

Concen: 0.77 ng

RT: 21.839 min Scan# 15

Delta R.T. -0.000 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:228 Resp: 15797

Ion Ratio Lower Upper

228 100

226 29.3 24.0 36.0

229 20.5 16.0 24.0

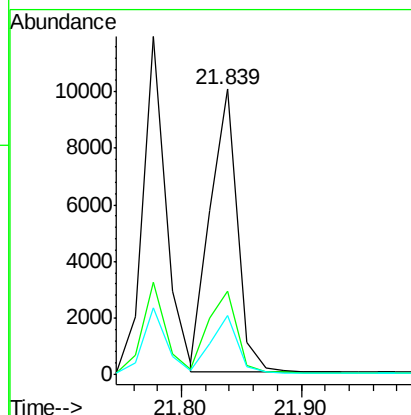

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.55 ng

RT: 21.652 min Scan# 1568

Delta R.T. -0.000 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:149 Resp: 26438


Ion Ratio Lower Upper

149 100

167 6.9 5.4 8.0

279 0.8 0.7 1.1


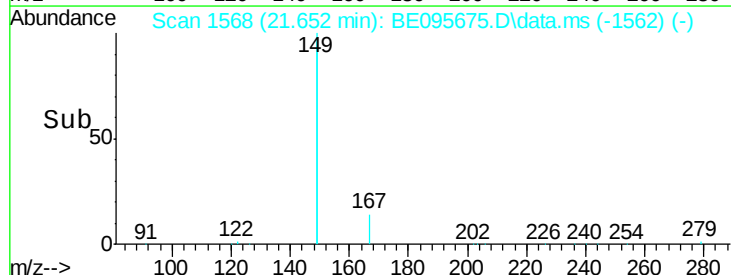
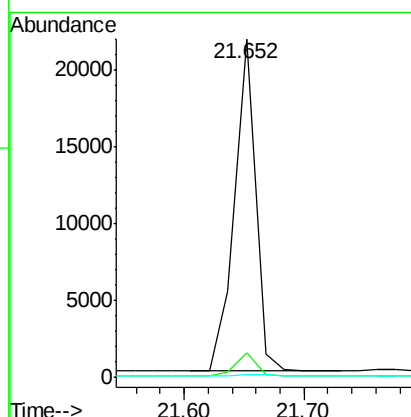





#33
 Indeno(1,2,3-cd)pyrene
 Concen: 0.78 ng
 RT: 27.229 min Scan# 2731
 Delta R.T. -0.000 min
 Lab File: BE095675.D
 Acq: 23 Feb 2018 10:17




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:276 Resp: 15473
 Ion Ratio Lower Upper
 276 100
 138 22.0 22.5 33.7#
 277 24.8 19.9 29.9

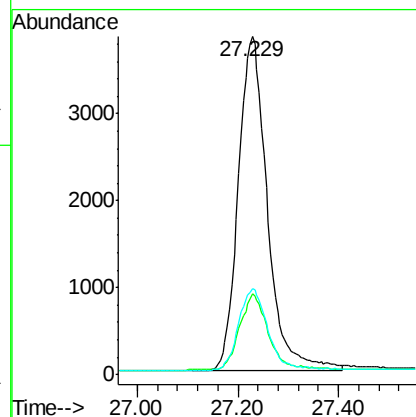

#34
 Perylene-d12
 Concen: 0.40 ng
 RT: 24.421 min Scan# 2116
 Delta R.T. -0.001 min
 Lab File: BE095675.D
 Acq: 23 Feb 2018 10:17

Tgt Ion:264 Resp: 5506
 Ion Ratio Lower Upper
 264 100
 260 26.6 20.5 30.7
 265 26.5 22.8 34.2

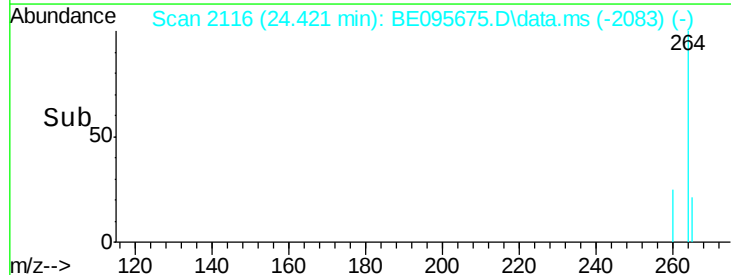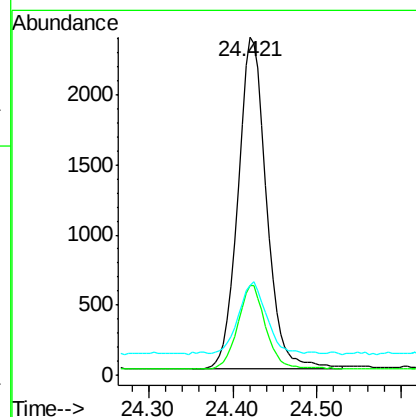



#35

Benzo(b)fluoranthene

Concen: 0.81 ng

RT: 23.605 min Scan# 1937

Delta R.T. -0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:252 Resp: 15181

Ion Ratio Lower Upper

252 100

253 22.4 20.0 30.0

125 10.6 16.0 24.0#

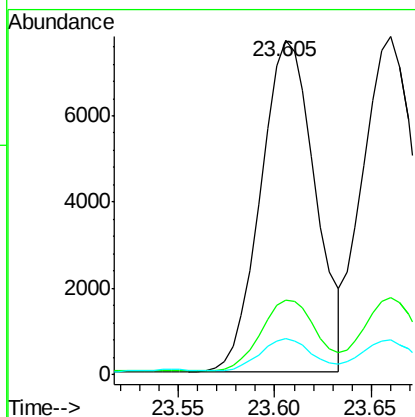

#36

Benzo(k)fluoranthene

Concen: 0.80 ng

RT: 23.660 min Scan# 1949

Delta R.T. -0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:252 Resp: 15434


Ion Ratio Lower Upper

252 100

253 22.9 16.0 24.0

125 10.4 8.0 12.0

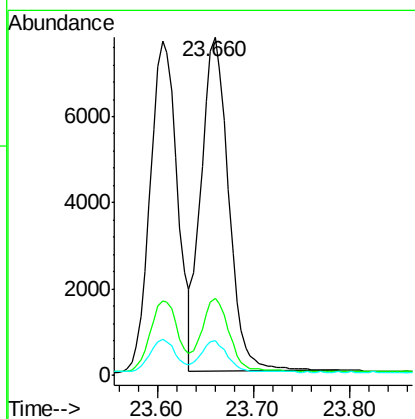

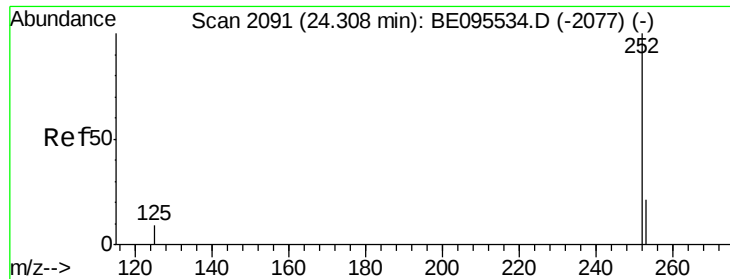

#37

Benzo(a)pyrene

Concen: 0.79 ng

RT: 24.302 min Scan# 2091

Delta R.T. -0.001 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :





Tot Ion:252 Resp: 13884

Ion Ratio Lower Upper

252 100

253 23.1 16.0 24.0

125 11.7 12.0 18.0#

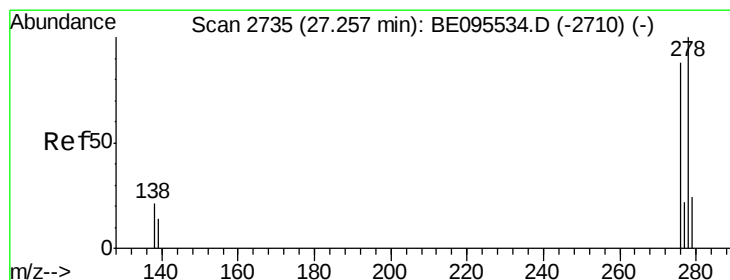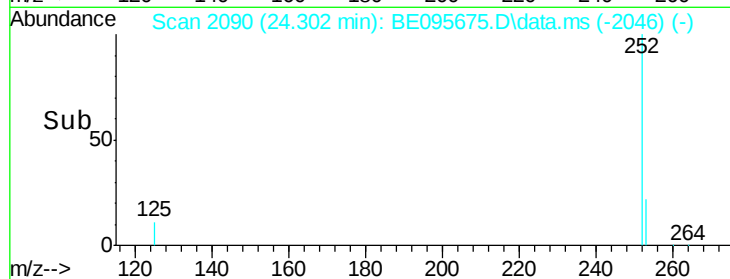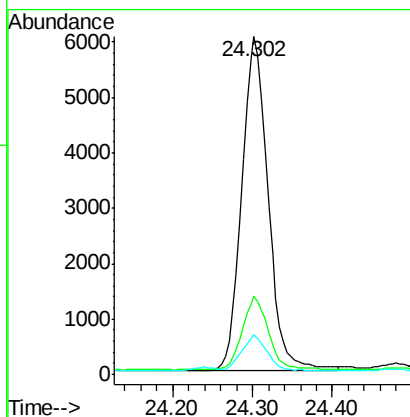

#38

Dibenzo(a,h)anthracene

Concen: 0.82 ng

RT: 27.247 min Scan# 2733

Delta R.T. -0.000 min

Lab File: BE095675.D

Acq: 23 Feb 2018 10:17




Tgt Ion:278 Resp: 12535


Ion Ratio Lower Upper

278 100

139 15.7 16.0 24.0#

279 24.8 20.0 30.0

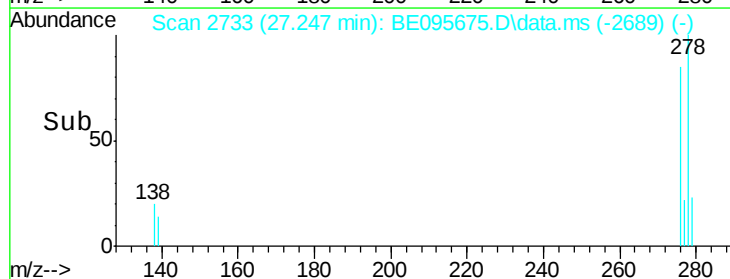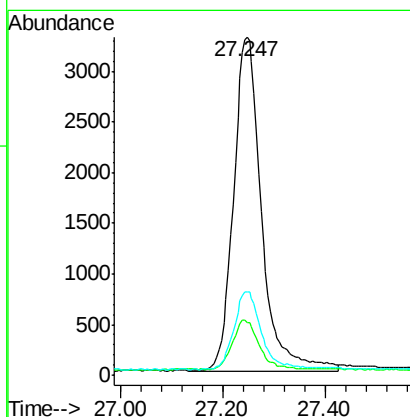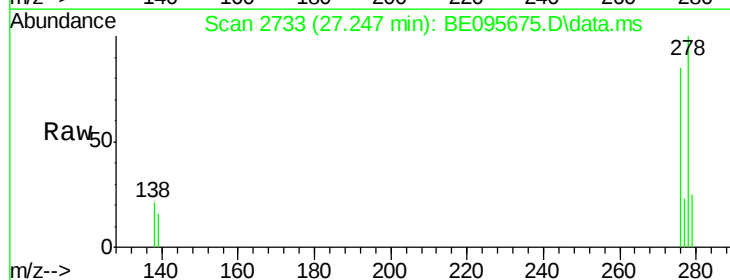

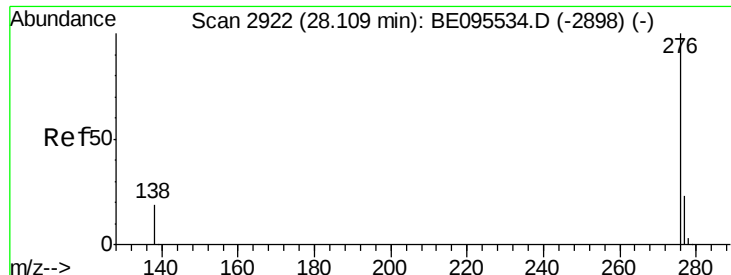

#39

Benzo(a,h,i)perylene

Concen: 0.80 ng

RT: 28.099 min Scan# 29

Delta R.T. -0.000 min


Lab File: BE095675.D

Acq: 23 Feb 2018 10:17

Instrument :

BNA_E

ClientSampleId :

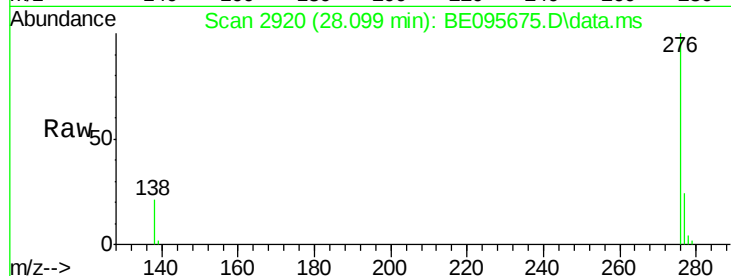

Tot Ion:	276	Resp:	13102
Ion Ratio	Lower	Upper	
276	100		
277	24.2	16.0	24.0#
138	21.2	20.0	30.0

