
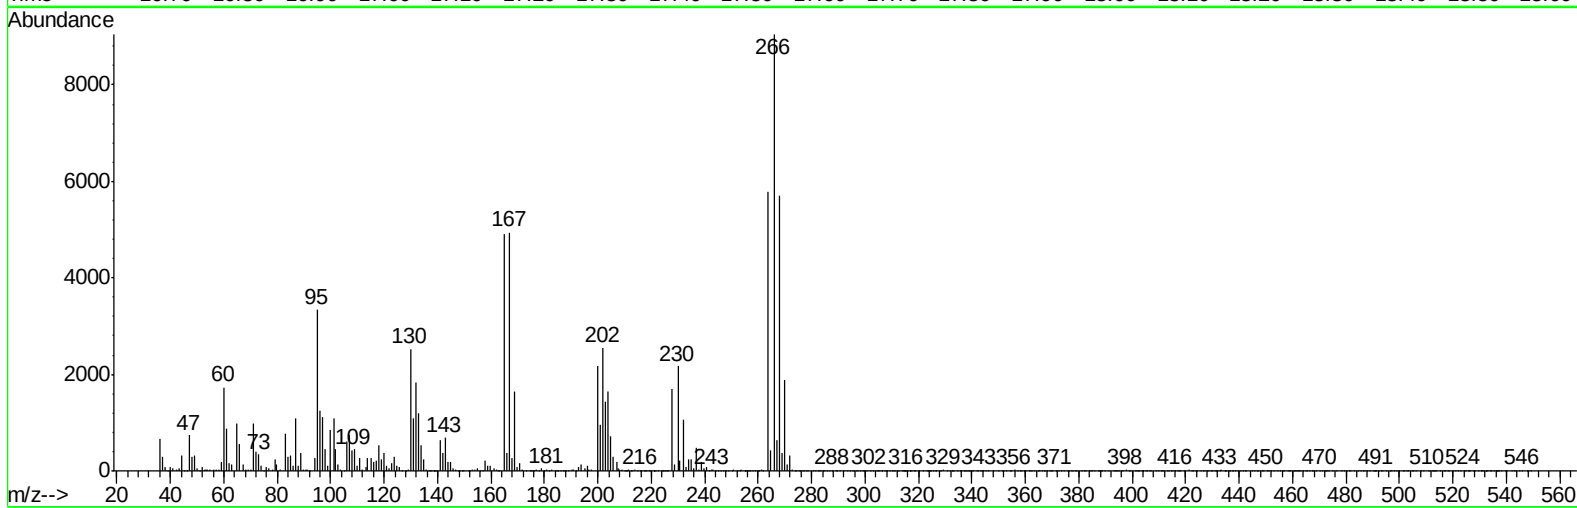


Data Path : Z:\HPCHEM1\BNA E\DATA\BE022318\
Data File : BE095671.D
Acq On : 23 Feb 2018 7:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 04:52:15 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 02:43:46 2018
Response via : Initial Calibration

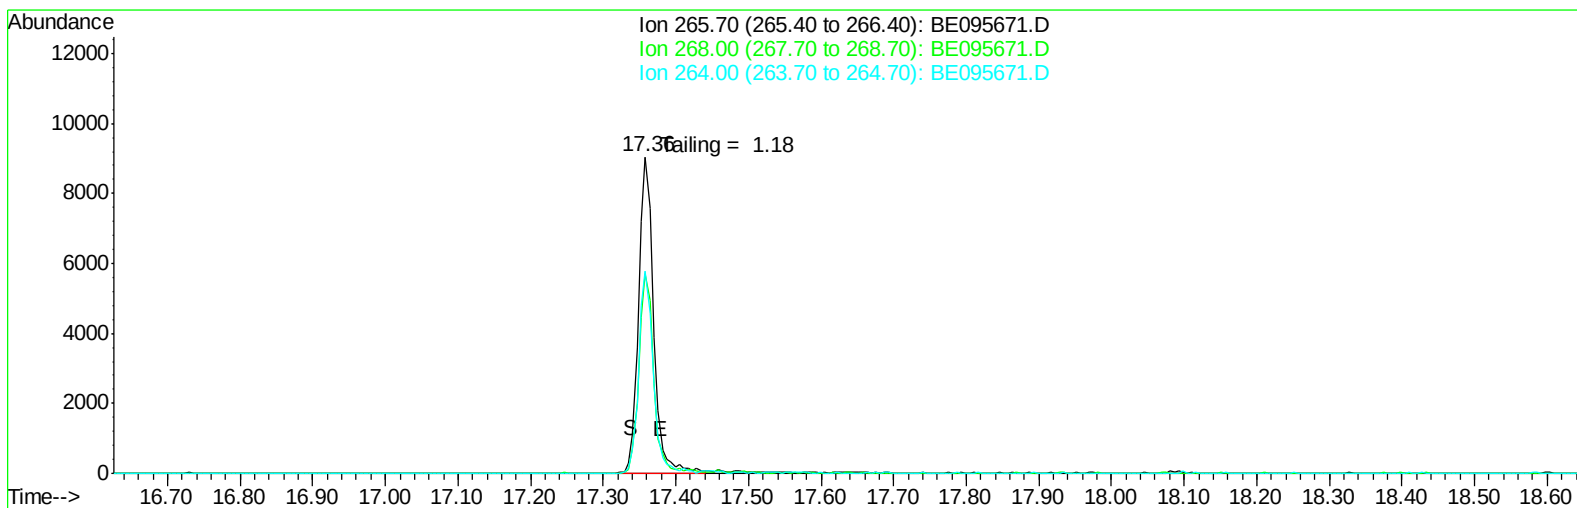

TIC: BE095671.D

(69) Pentachlorophenol (C)



17.358min (+6.148) 238890.11ng m

response 13060

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.08
264.00	61.90	64.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE022318\
Data File : BE095671.D
Acq On : 23 Feb 2018 7:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 04:52:15 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 02:43:46 2018
Response via : Initial Calibration

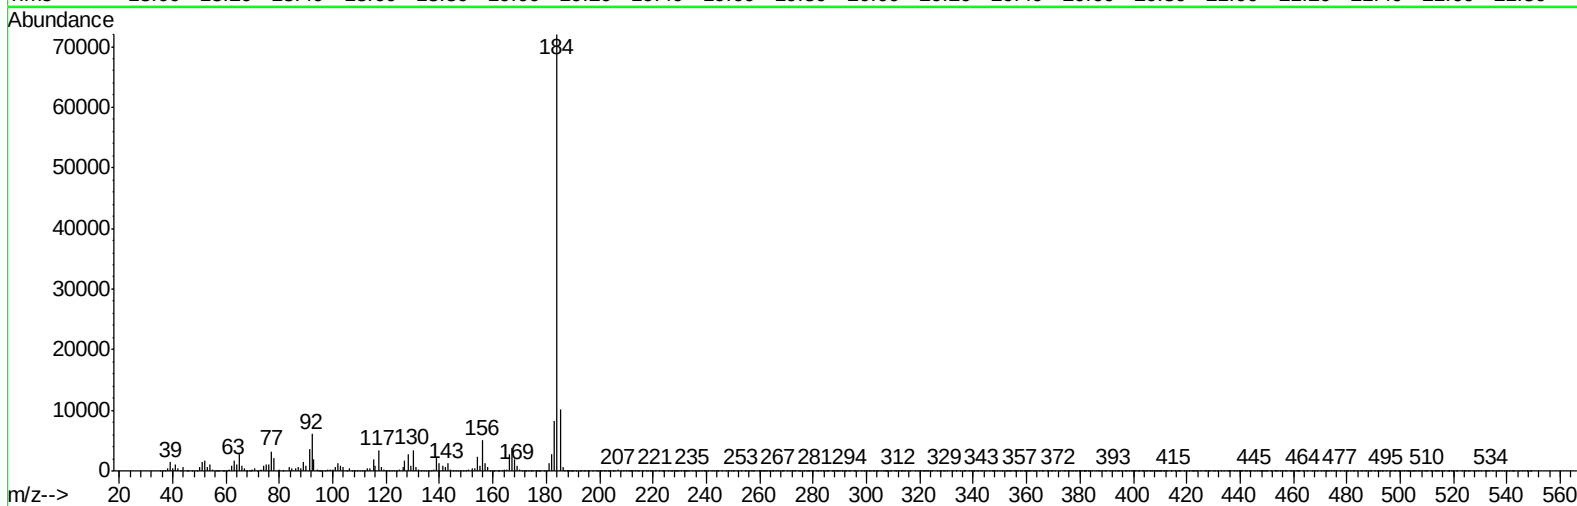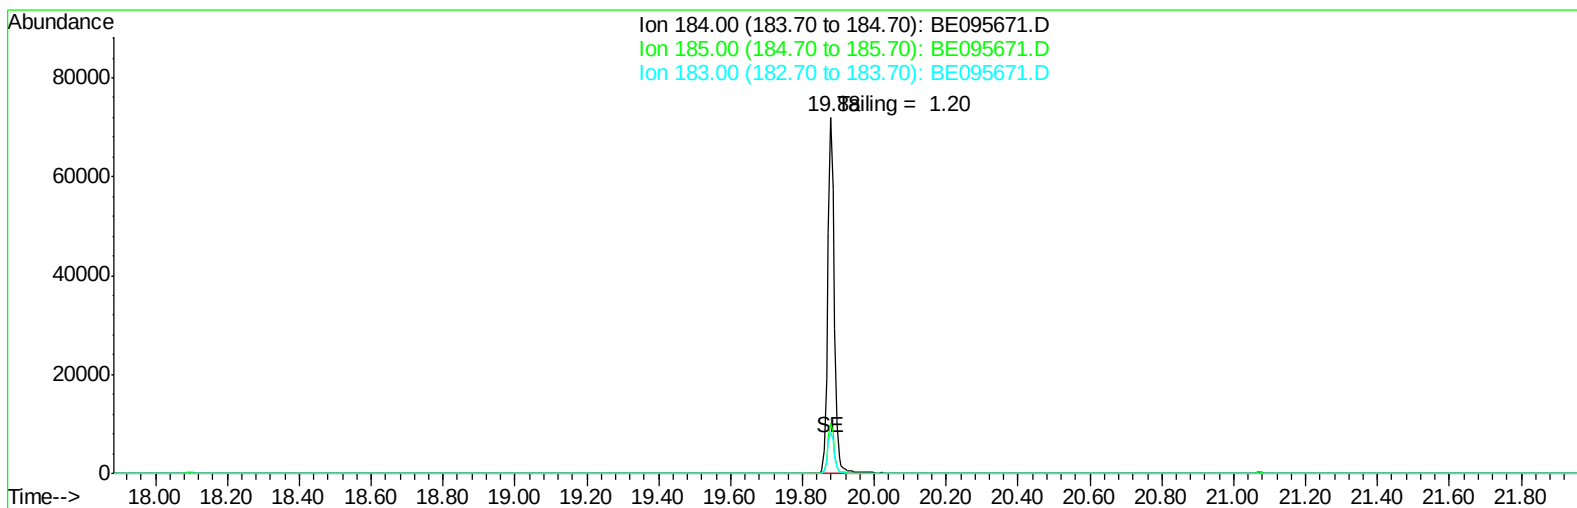

TIC: BE095671.D

(76) Benzidine

19.879min (+7.140) 338468.12ng m

response 88576

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.01
183.00	11.60	11.45
0.00	0.00	0.00