


Data Path : Z:\HPCHEM1\BNA E\DATA\BE022318\
Data File : BE095671.D
Acq On : 23 Feb 2018 7:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE022318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 23 12:12:42 2018

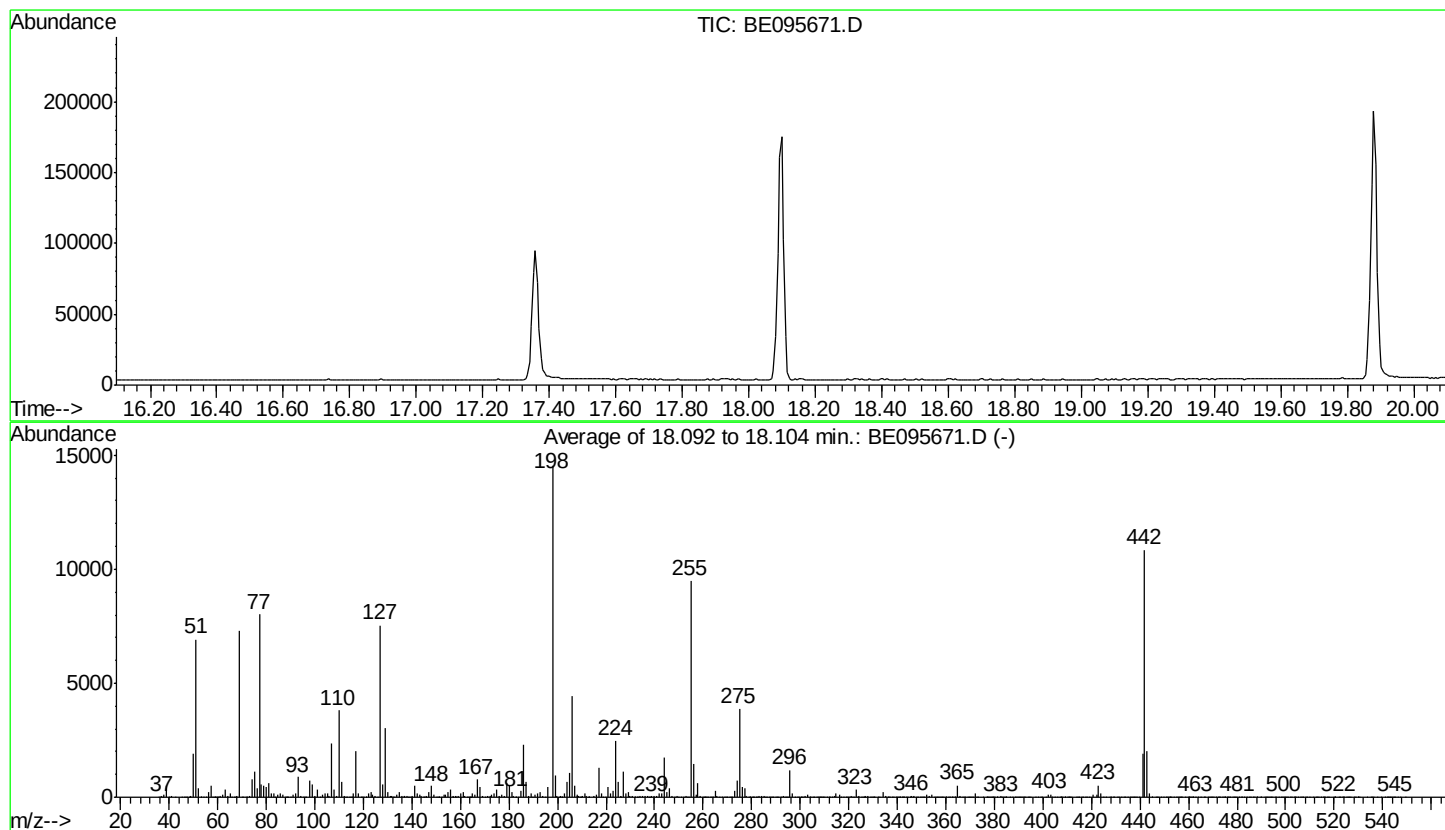

AutoFind: Scans 2639, 2640, 2641; Background Corrected with Scan 2630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.6	6917	PASS
68	69	0.00	2	0.4	32	PASS
69	198	0.00	100	50.3	7316	PASS
70	69	0.00	2	0.3	21	PASS
127	198	10	80	51.8	7541	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14544	PASS
199	198	5	9	6.6	967	PASS
275	198	10	60	26.7	3879	PASS
365	198	1	100	3.5	513	PASS
441	442	0.01	24	17.8	1926	PASS
442	198	50	100	74.5	10842	PASS
443	442	15	24	18.5	2003	PASS