


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE022415\
 Data File : BE089683.D
 Acq On : 24 Feb 2015 22:49
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 25 04:05:13 2015

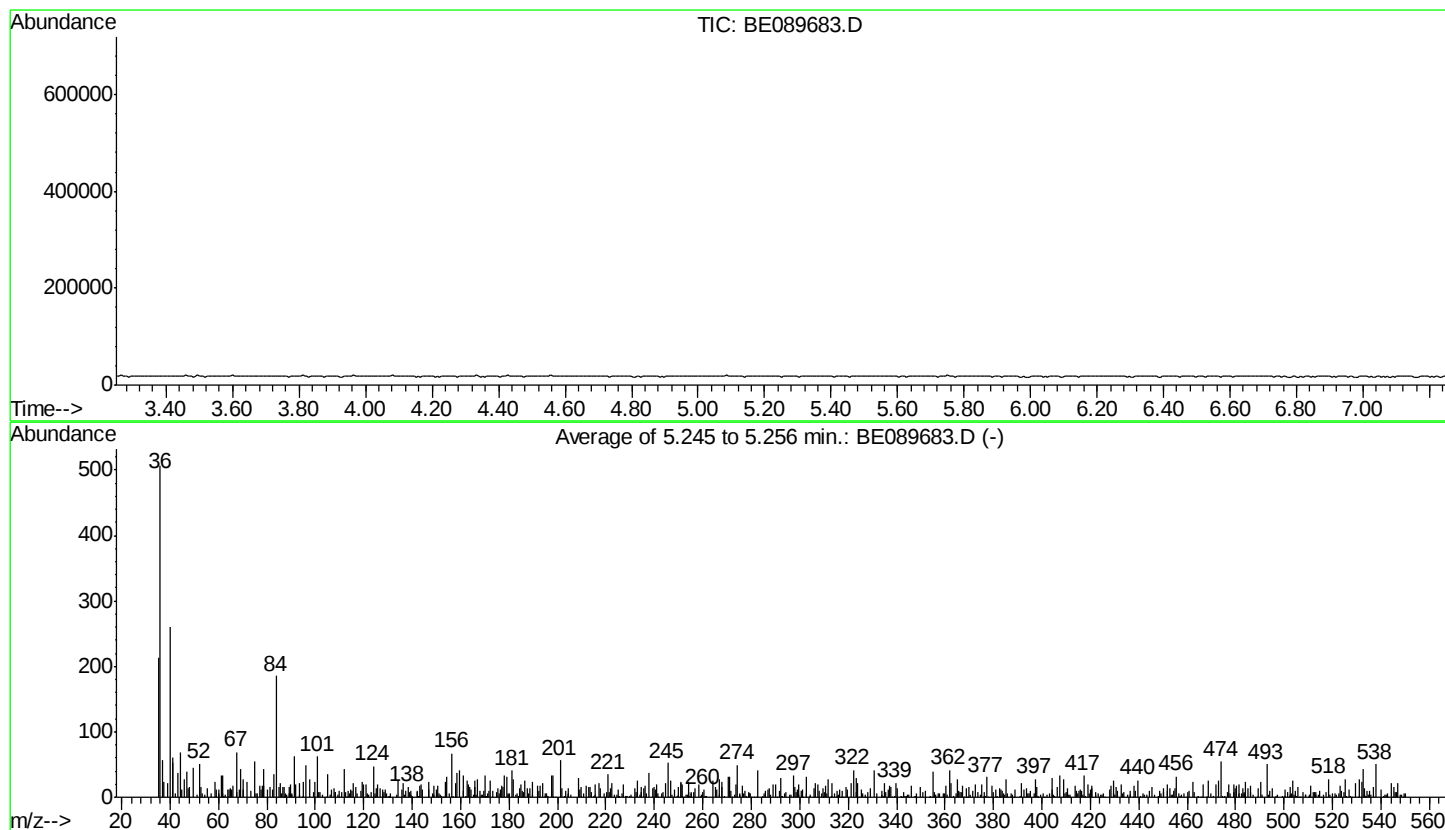

AutoFind: Scans 656, 657, 658; Background Corrected with Scan 650

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	8.8	3	FAIL*
68	69	0.00	2	27.9	12	FAIL*
69	198	0.00	100	126.5	43	FAIL*
70	69	0.00	2	65.1	28	FAIL*
127	198	10	80	41.2	14	PASS
197	198	0.00	2	97.1	33	FAIL*
198	198	100	100	100.0	34	PASS
199	198	5	9	2.9	1	FAIL*
275	198	10	60	17.6	6	PASS
365	198	1	100	82.4	28	PASS
441	442	0.01	24	100.0	5	FAIL*
442	198	50	100	14.7	5	FAIL*
443	442	15	24	80.0	4	FAIL*