


Data Path : Z:\HPCHEM1\BNA_E\Data\BE022415\
 Data File : BE089665.D
 Acq On : 24 Feb 2015 10:55
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 24 17:00:09 2015

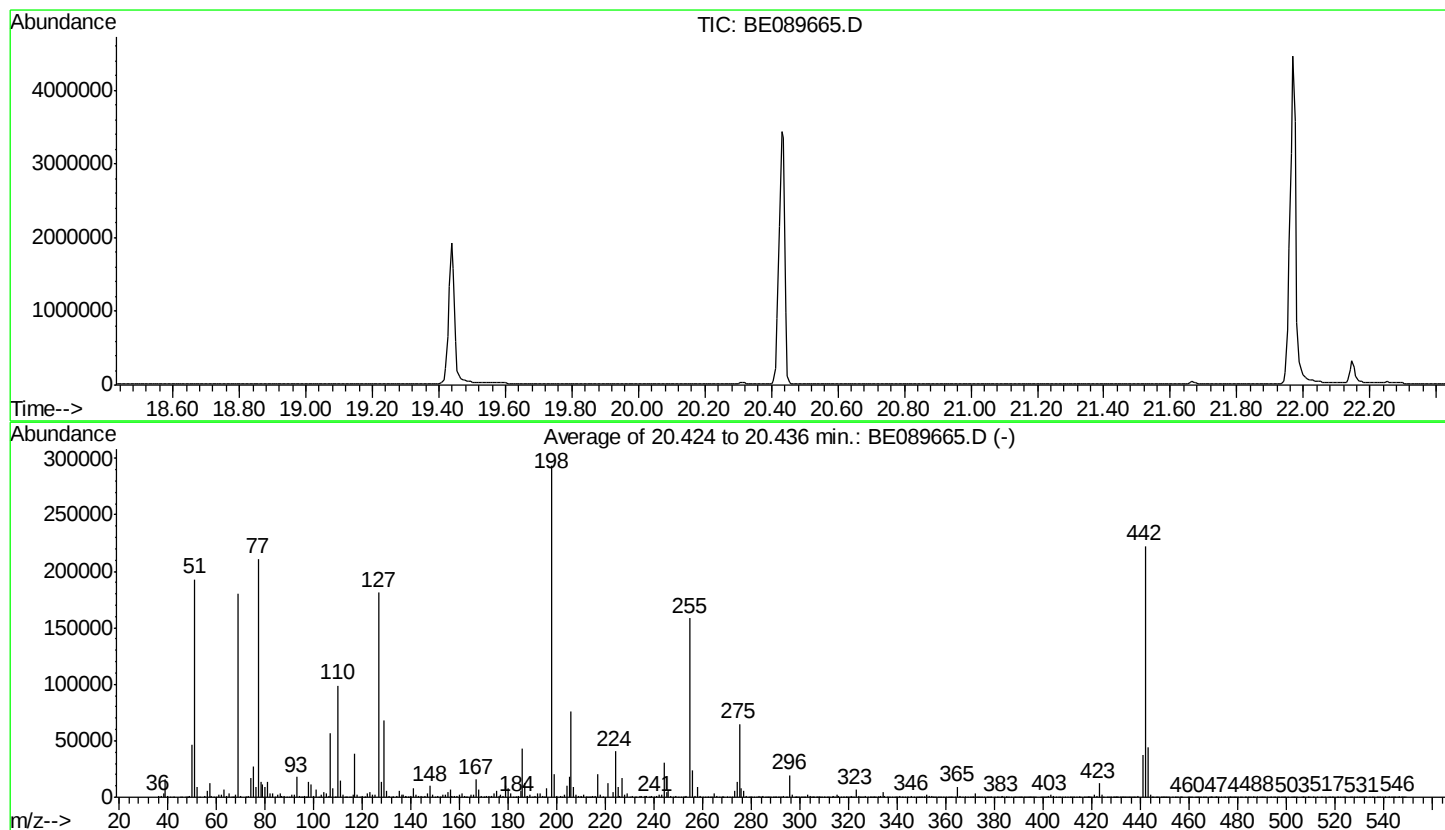

AutoFind: Scans 3240, 3241, 3242; Background Corrected with Scan 3233

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.7	192946	PASS
68	69	0.00	2	1.3	2294	PASS
69	198	0.00	100	61.4	180309	PASS
70	69	0.00	2	0.6	1064	PASS
127	198	10	80	61.7	181169	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	293568	PASS
199	198	5	9	6.8	19899	PASS
275	198	10	60	22.0	64674	PASS
365	198	1	100	3.2	9539	PASS
441	442	0.01	24	16.9	37550	PASS
442	198	50	100	75.7	222184	PASS
443	442	15	24	20.0	44416	PASS