
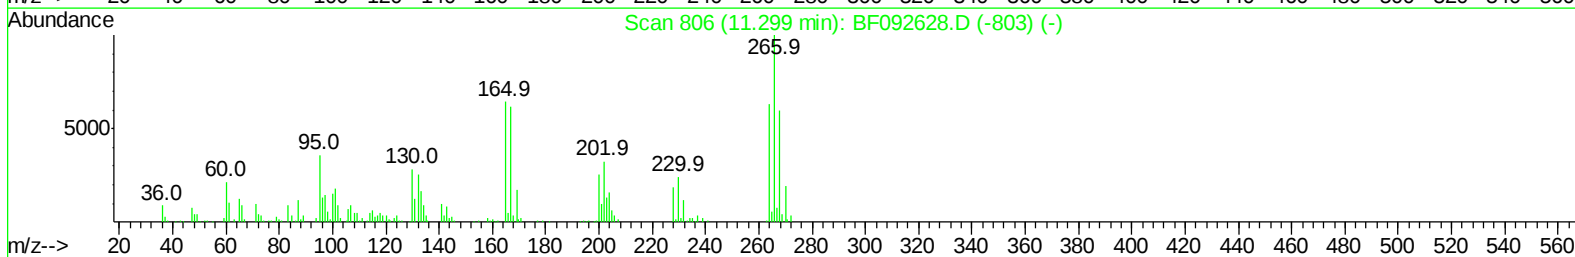
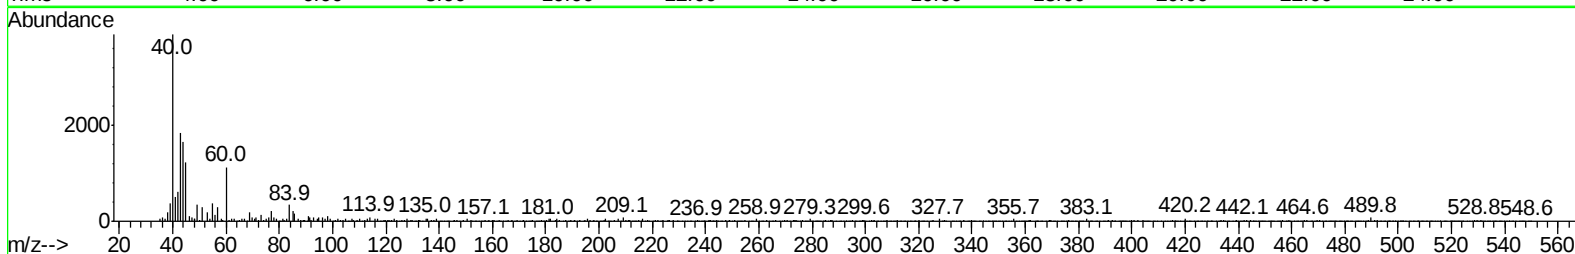


Data Path : Z:\HPCHEM1\BNA E\Data\BE022417\
Data File : BE092754.D
Acq On : 24 Feb 2017 11:17
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 17:56:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

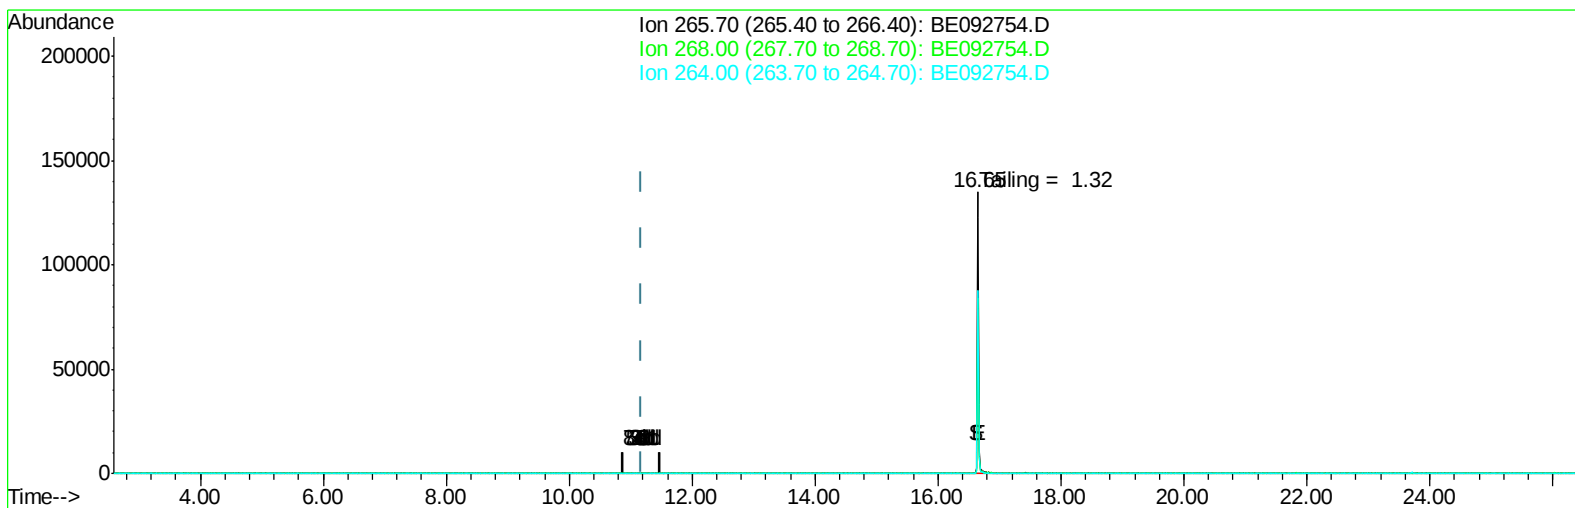

TIC: BE092754.D

(69) Pentachlorophenol (C)




11.383min (+0.198) 177.94ng

response 28

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	76.92
264.00	62.90	69.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE022417\
Data File : BE092754.D
Acq On : 24 Feb 2017 11:17
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 17:56:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

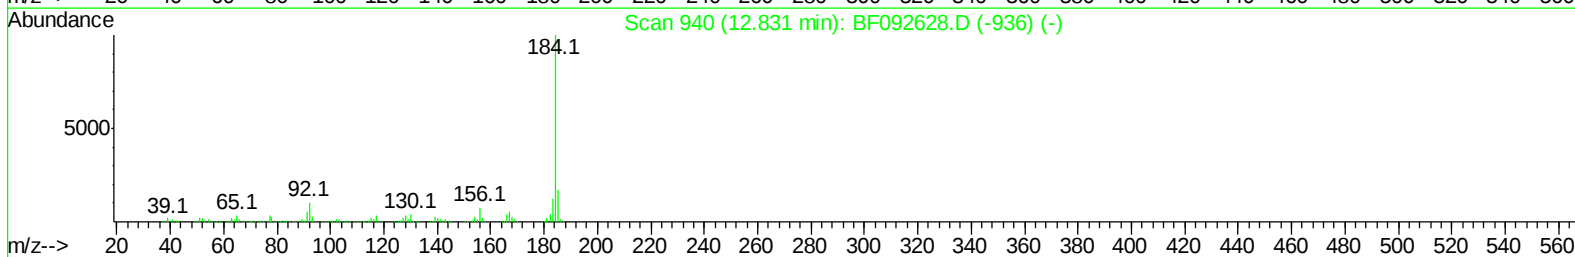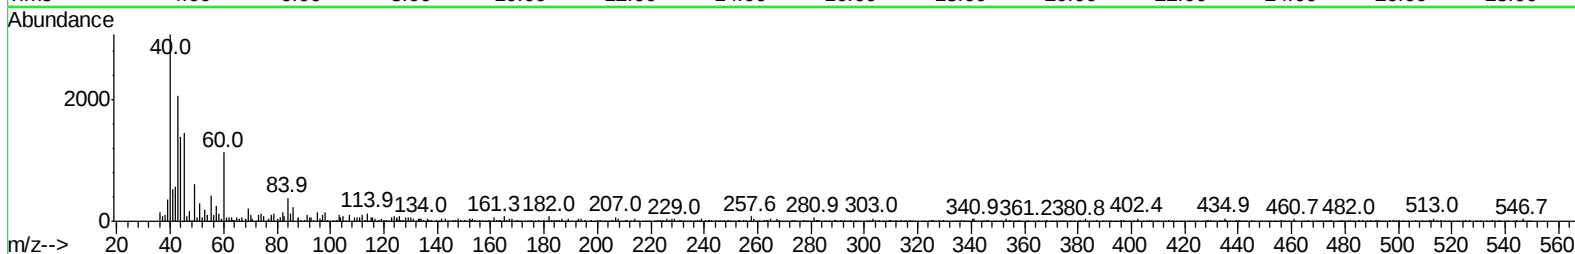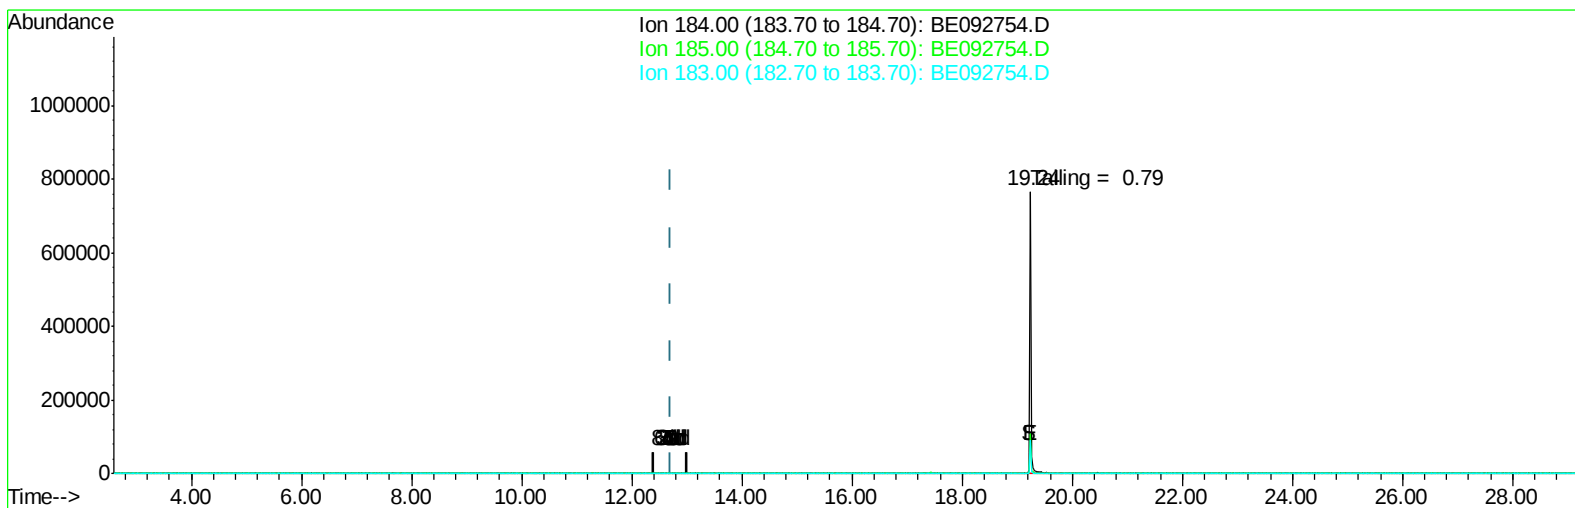

TIC: BE092754.D

(76) Benzidine

12.728min (+0.011) 18.61ng

response 23

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	0.00#
183.00	11.50	53.19#
0.00	0.00	0.00