


Data Path : Z:\HPCHEM1\BNA E\DATA\BE022417\
 Data File : BE092754.D
 Acq On : 24 Feb 2017 11:17
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE021517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 15 17:05:20 2017

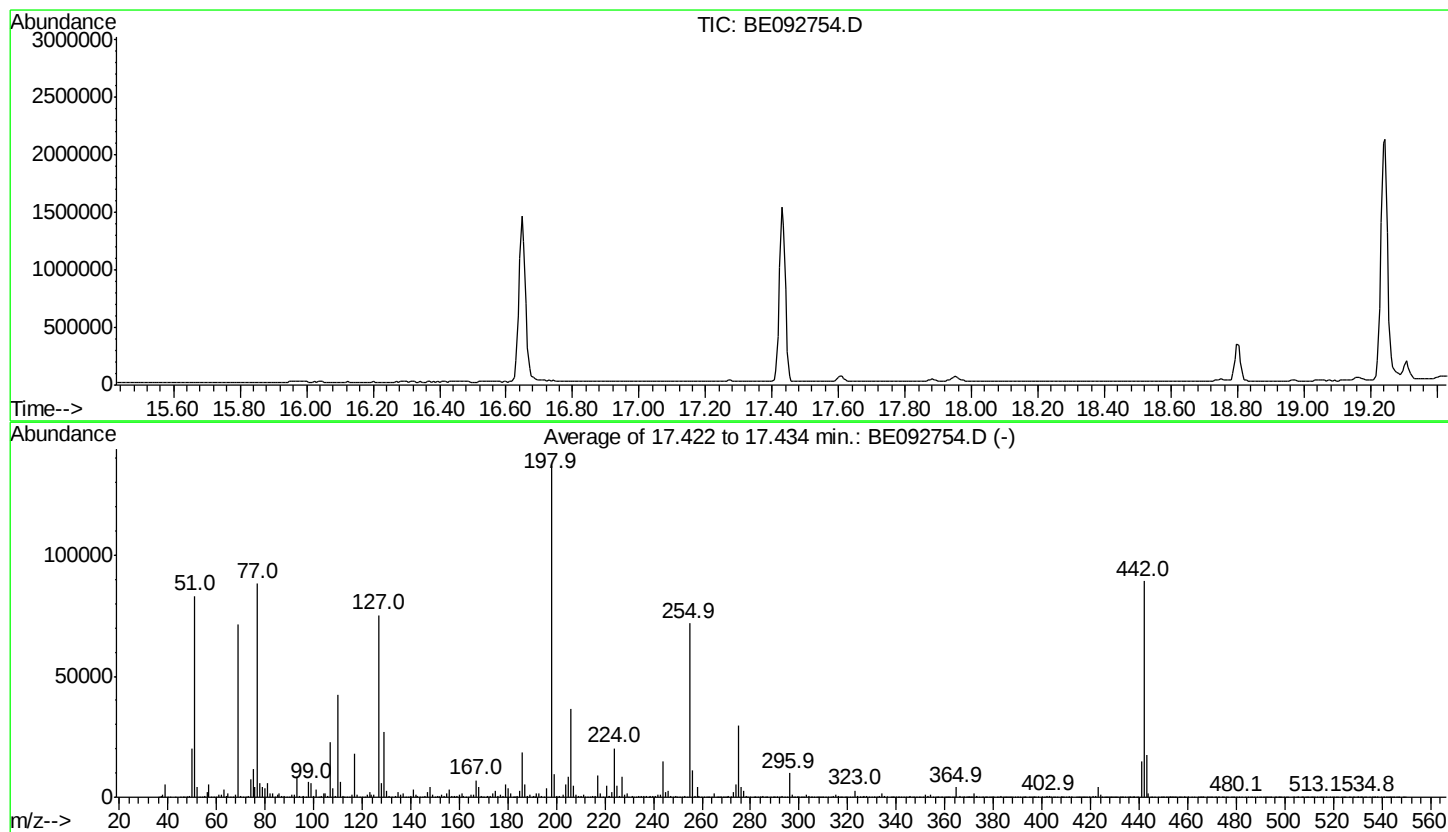

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.7	83206	PASS
68	69	0.00	2	1.4	976	PASS
69	198	0.00	100	52.2	71550	PASS
70	69	0.00	2	0.4	316	PASS
127	198	10	80	55.0	75420	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	137088	PASS
199	198	5	9	6.8	9302	PASS
275	198	10	60	21.7	29815	PASS
365	198	1	100	3.1	4198	PASS
441	442	0.01	24	16.8	14983	PASS
442	198	50	100	65.1	89254	PASS
443	442	15	24	19.7	17615	PASS