


Data Path : Z:\HPCHEM1\BNA_E\Data\BE022515\
 Data File : BE089683.D
 Acq On : 25 Feb 2015 15:37
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 25 14:06:35 2015

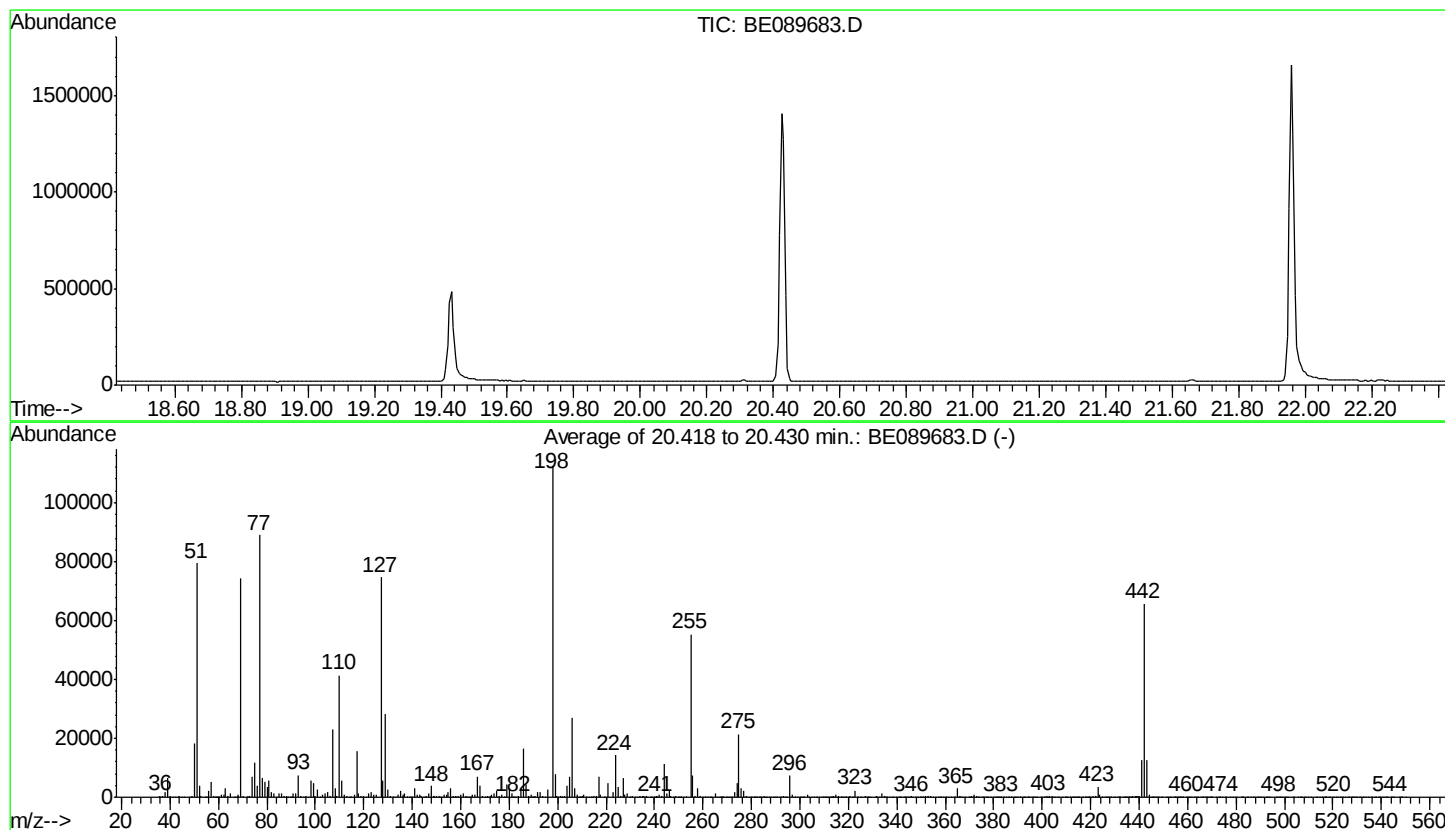

AutoFind: Scans 3239, 3240, 3241; Background Corrected with Scan 3232

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	70.6	79430	PASS
68	69	0.00	2	1.0	770	PASS
69	198	0.00	100	66.2	74495	PASS
70	69	0.00	2	0.5	348	PASS
127	198	10	80	66.4	74691	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	112565	PASS
199	198	5	9	6.9	7754	PASS
275	198	10	60	19.1	21503	PASS
365	198	1	100	2.7	3033	PASS
441	442	0.01	24	19.0	12525	PASS
442	198	50	100	58.4	65755	PASS
443	442	15	24	19.4	12777	PASS