


Data Path : Z:\HPCHEM1\BNA_E\Data\BE022615\
 Data File : BE089691.D
 Acq On : 26 Feb 2015 11:06
 Operator : TP/JJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIMPAH-BE022415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 25 14:06:35 2015

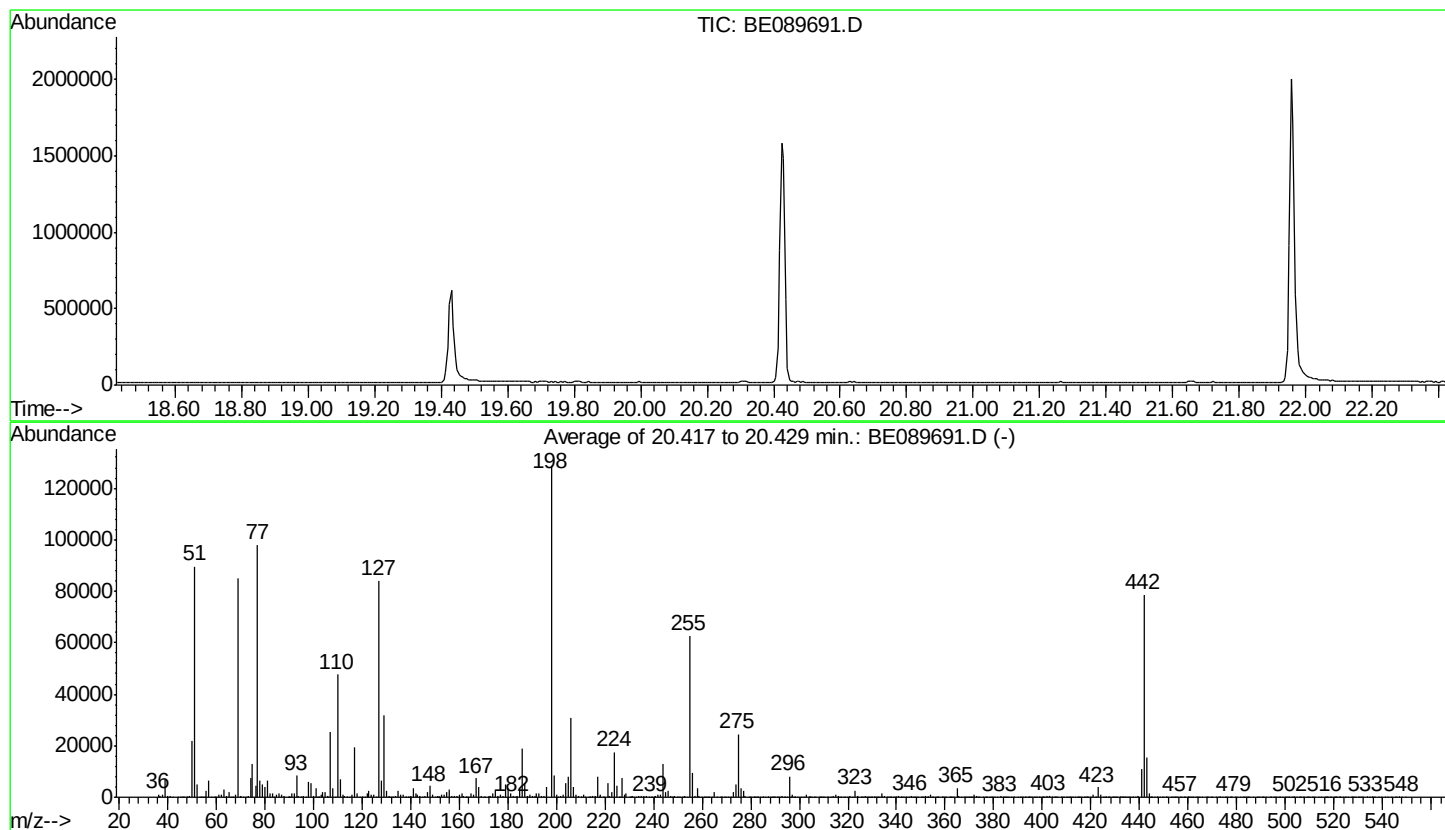

AutoFind: Scans 3239, 3240, 3241; Background Corrected with Scan 3230

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	69.5	89493	PASS
68	69	0.00	2	1.4	1223	PASS
69	198	0.00	100	66.0	85033	PASS
70	69	0.00	2	0.3	290	PASS
127	198	10	80	65.4	84224	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	128770	PASS
199	198	5	9	6.5	8366	PASS
275	198	10	60	19.0	24472	PASS
365	198	1	100	2.8	3594	PASS
441	442	0.01	24	13.7	10777	PASS
442	198	50	100	61.0	78592	PASS
443	442	15	24	19.5	15291	PASS