


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE022615\
Data File : BE089699.D
Acq On : 26 Feb 2015 20:12
Operator : TP/JJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE022615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 27 05:11:47 2015

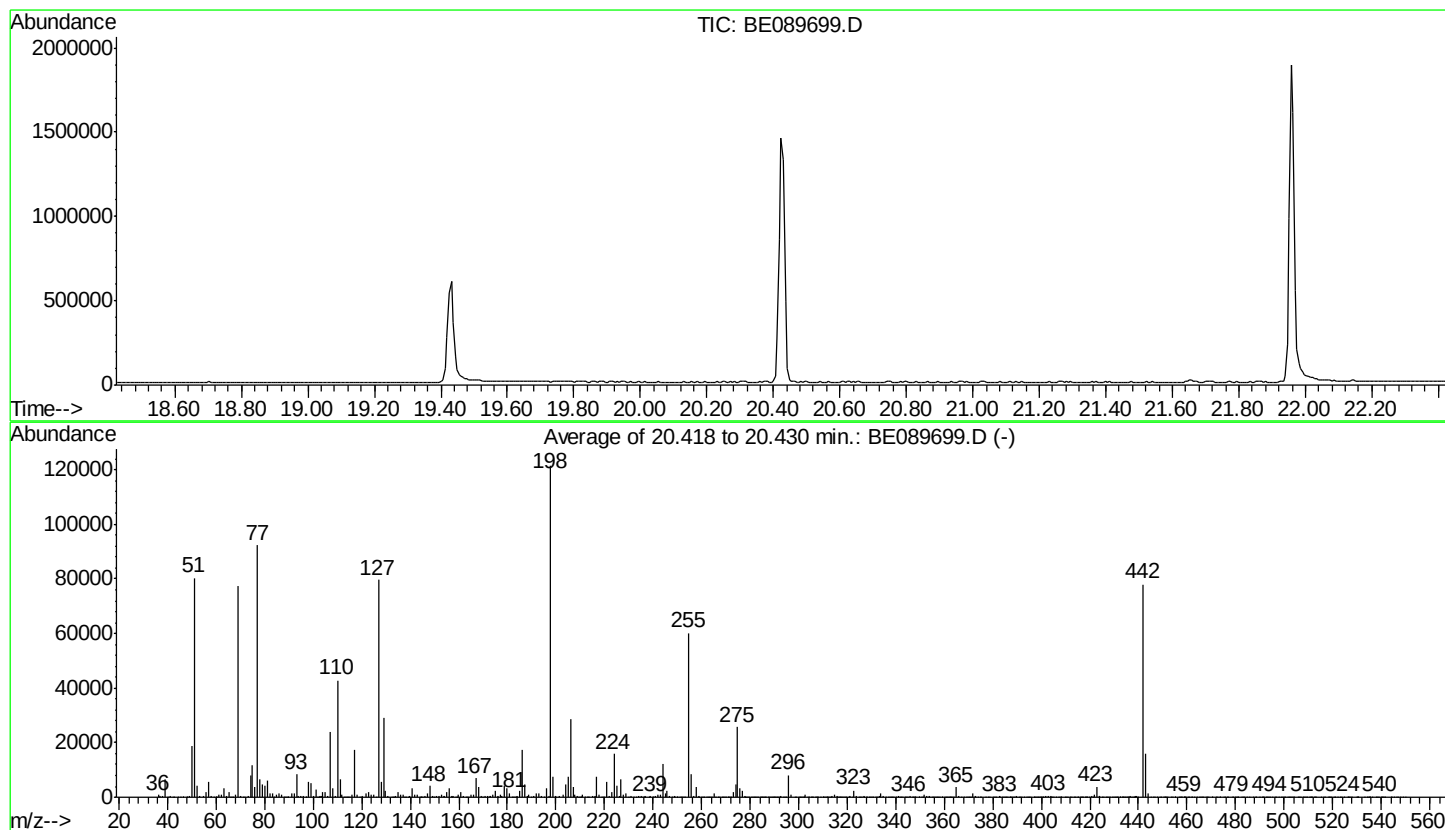

AutoFind: Scans 3239, 3240, 3241; Background Corrected with Scan 3228

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	66.2	80425	PASS
68	69	0.00	2	1.5	1181	PASS
69	198	0.00	100	63.6	77298	PASS
70	69	0.00	2	0.6	426	PASS
127	198	10	80	65.5	79634	PASS
197	198	0.00	2	0.2	264	PASS
198	198	100	100	100.0	121512	PASS
199	198	5	9	6.3	7684	PASS
275	198	10	60	21.1	25652	PASS
365	198	1	100	3.0	3599	PASS
441	442	0.01	24	0.0	0	FAIL *
442	198	50	100	64.2	78053	PASS
443	442	15	24	20.2	15785	PASS