


Data Path : Z:\HPCHEM1\BNA_E\Data\BE022615\
Data File : BE089699.D
Acq On : 26 Feb 2015 20:51
Operator : TP/JJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE022615.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 27 13:38:44 2015

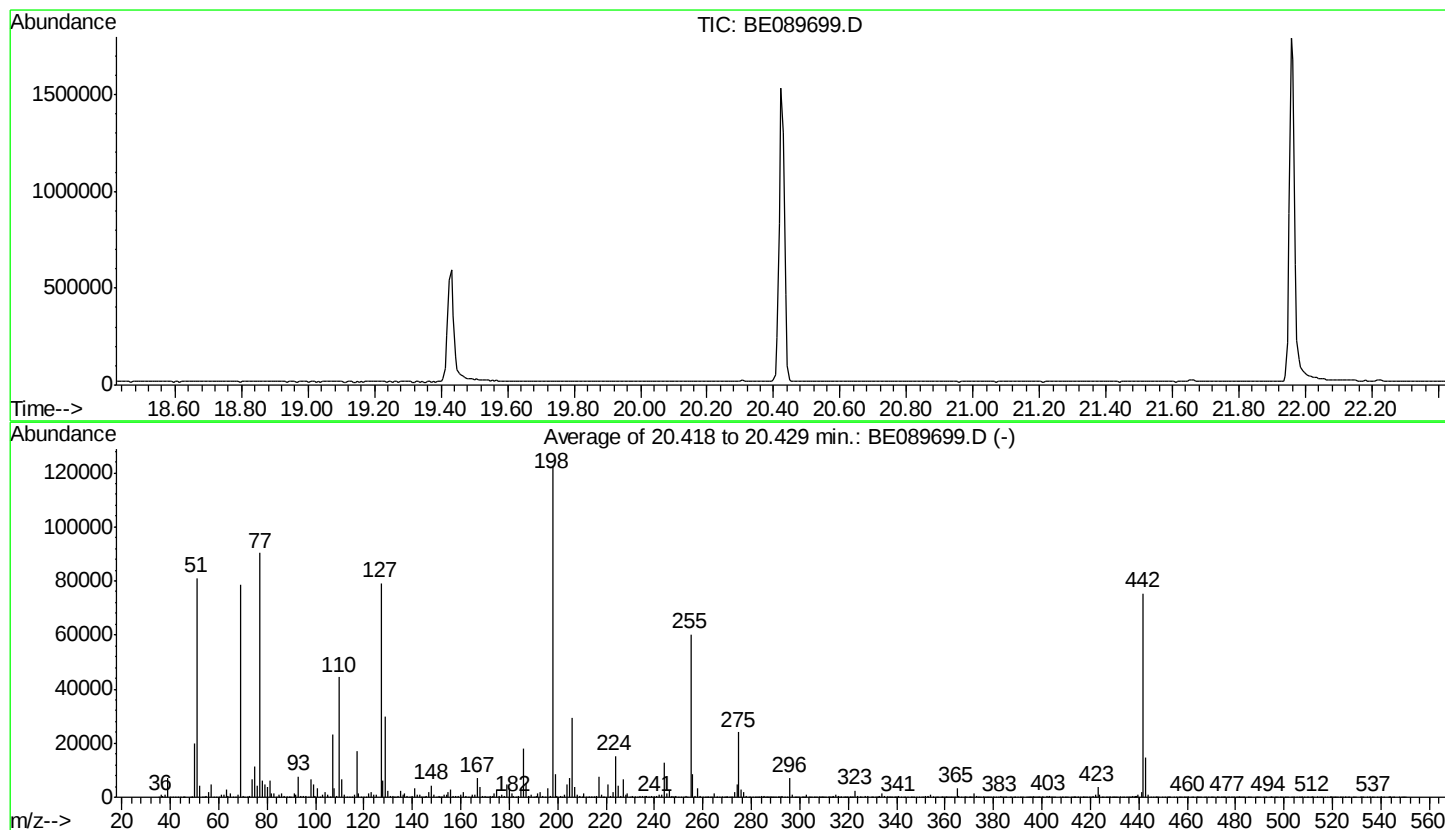

AutoFind: Scans 3239, 3240, 3241; Background Corrected with Scan 3230

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	66.1	80992	PASS
68	69	0.00	2	1.4	1066	PASS
69	198	0.00	100	64.0	78451	PASS
70	69	0.00	2	0.5	393	PASS
127	198	10	80	64.6	79246	PASS
197	198	0.00	2	0.4	479	PASS
198	198	100	100	100.0	122616	PASS
199	198	5	9	6.8	8388	PASS
275	198	10	60	19.6	24039	PASS
365	198	1	100	2.8	3407	PASS
441	442	0.01	24	2.8	2146	PASS
442	198	50	100	61.5	75376	PASS
443	442	15	24	19.7	14850	PASS