
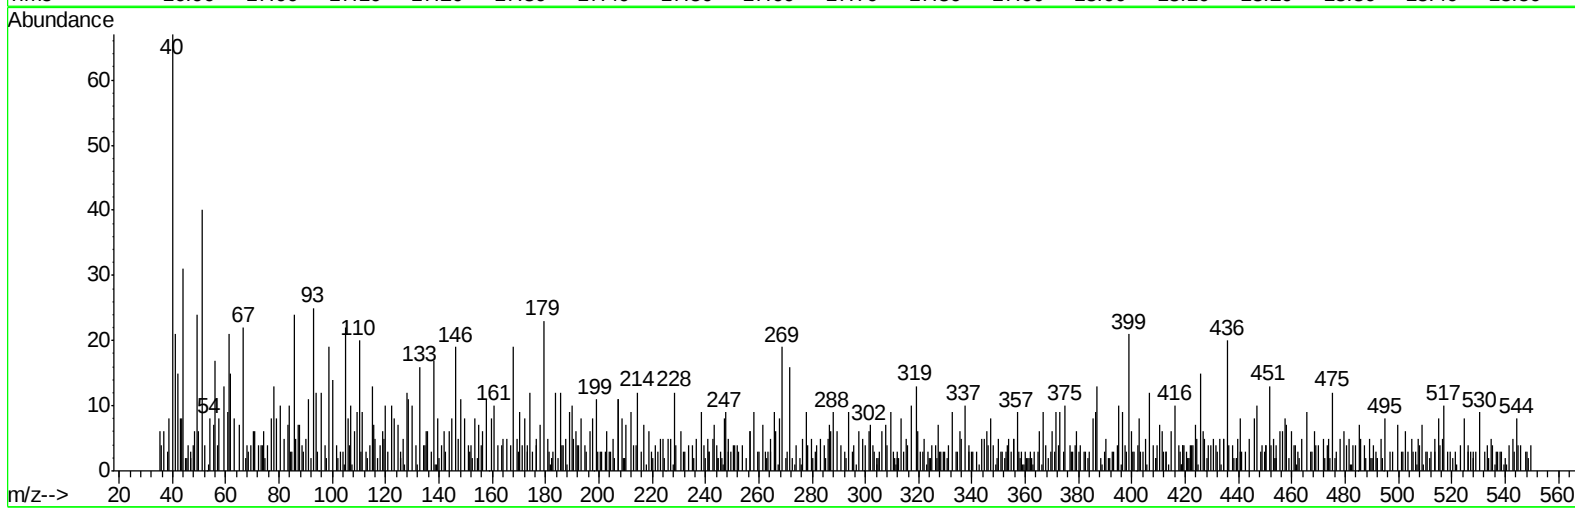


Data Path : Z:\HPCHEM1\BNA E\DATA\BE022618\
Data File : BE095687.D
Acq On : 26 Feb 2018 14:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 01:03:48 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 02:43:46 2018
Response via : Initial Calibration

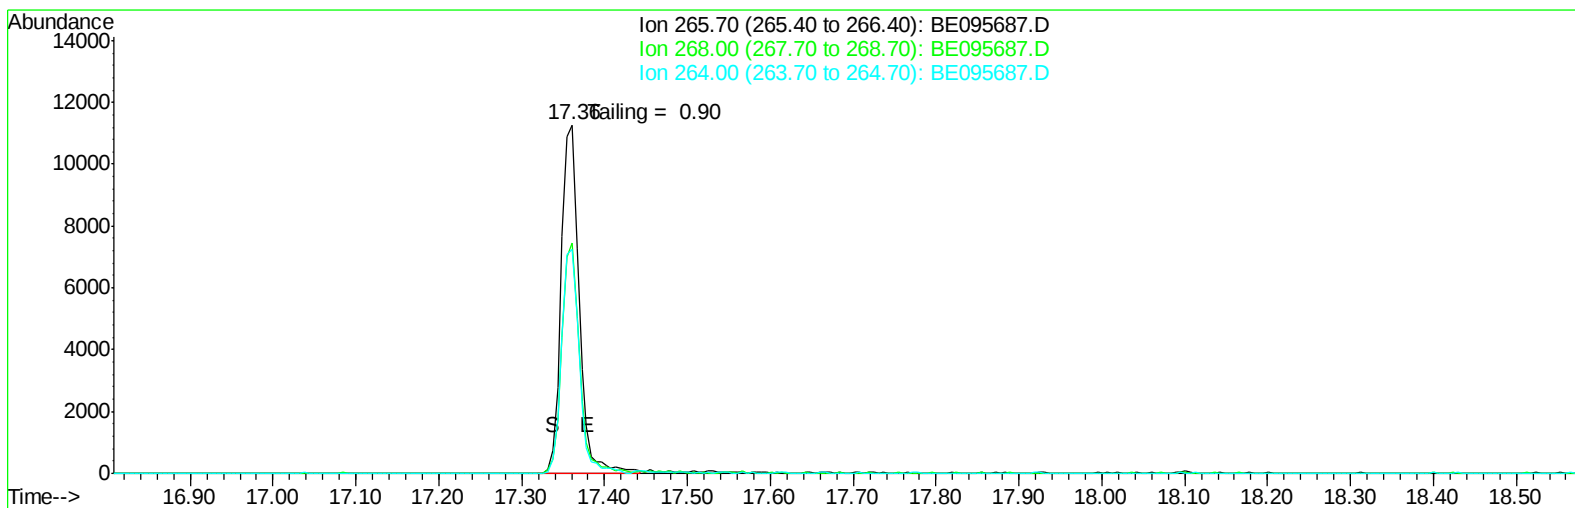

TIC: BE095687.D

(69) Pentachlorophenol (C)



11.250min (+0.040) 235.18ng

response 18

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	53.33
264.00	61.90	53.33
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE022618\
Data File : BE095687.D
Acq On : 26 Feb 2018 14:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 01:03:48 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 02:43:46 2018
Response via : Initial Calibration

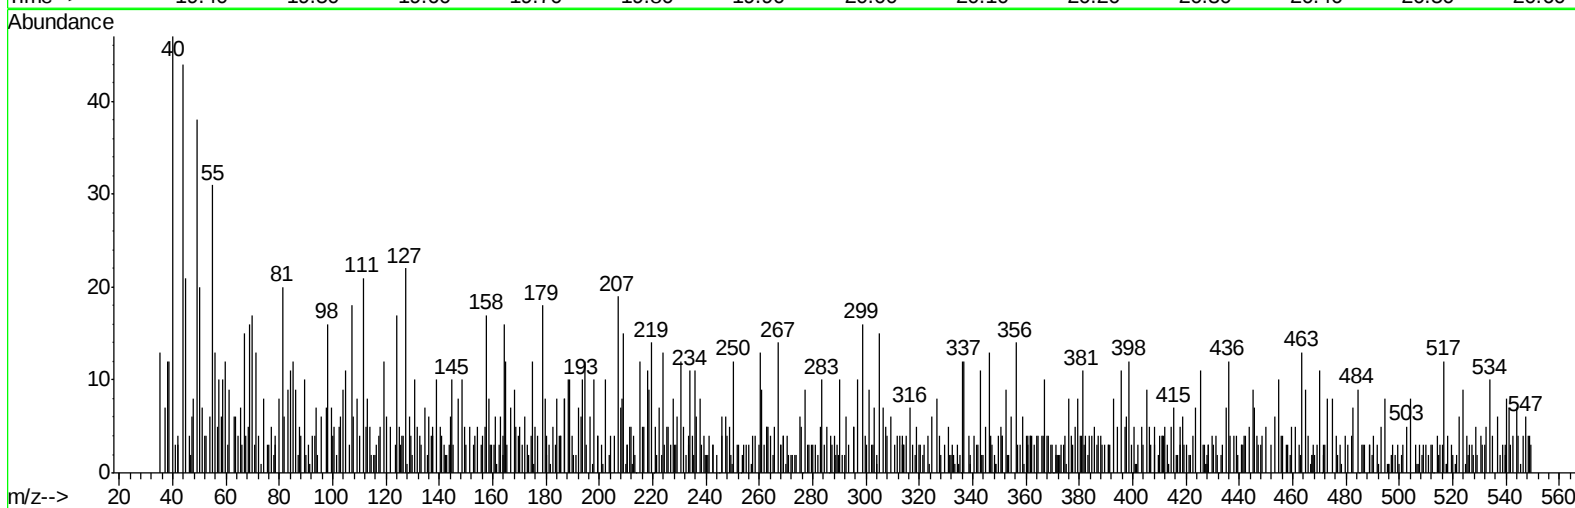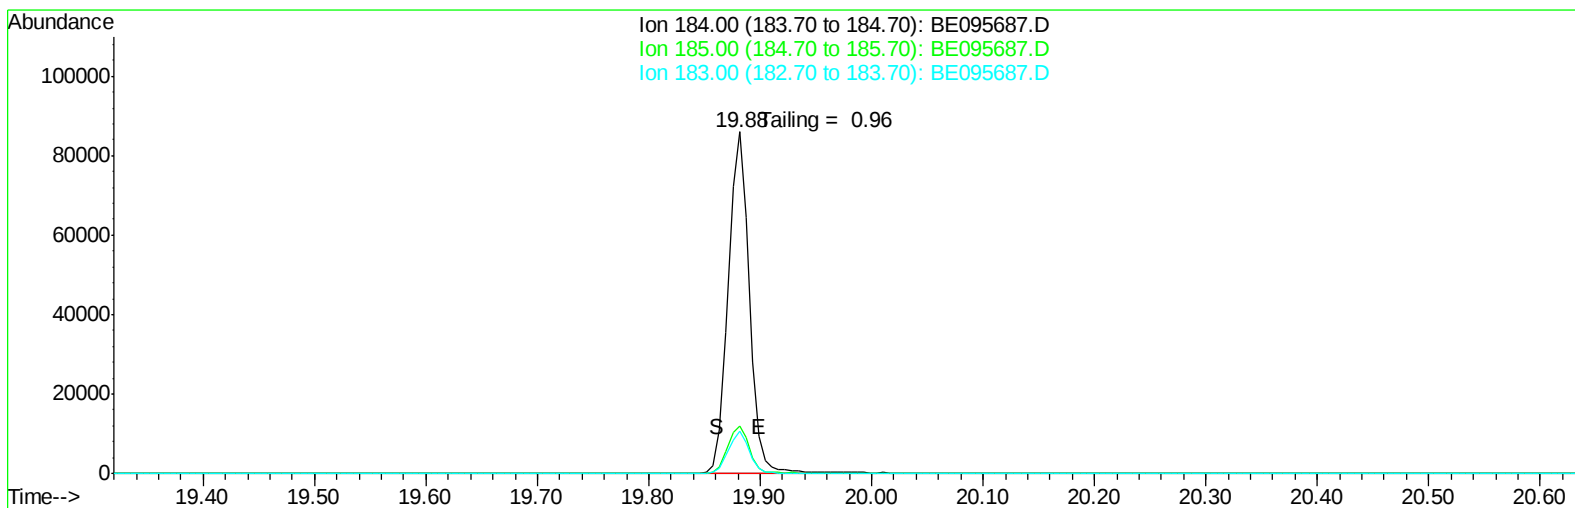

TIC: BE095687.D

(76) Benzidine

12.649min (-0.090) 74.90ng

response 14

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	150.00#
183.00	11.60	100.00#
0.00	0.00	0.00