


Data Path : Z:\HPCHEM1\BNA E\Data\BE022618\
Data File : BE095687.D
Acq On : 26 Feb 2018 14:06
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE022318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 23 12:12:42 2018

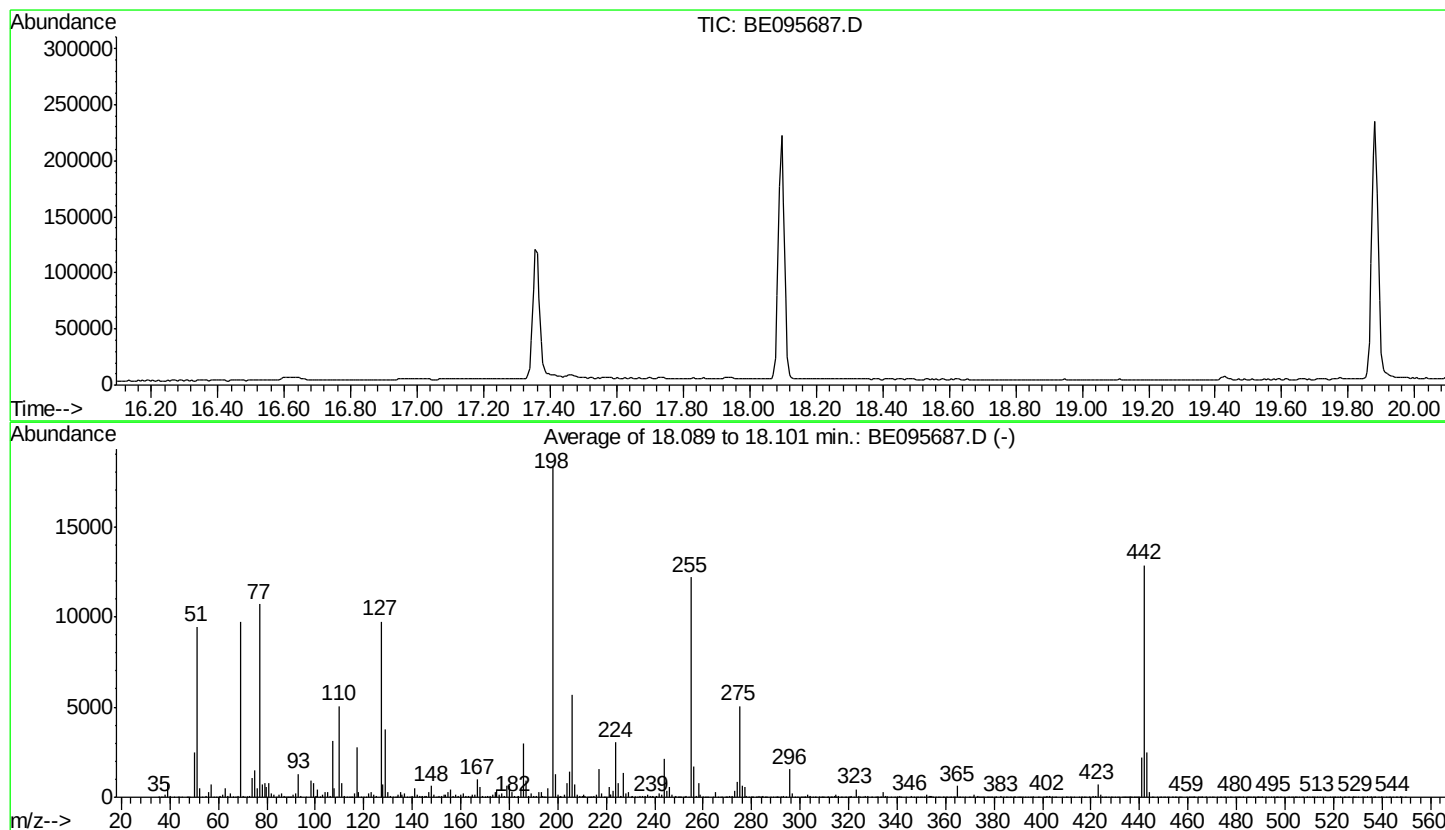

AutoFind: Scans 2638, 2639, 2640; Background Corrected with Scan 2630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.5	9456	PASS
68	69	0.00	2	0.5	49	PASS
69	198	0.00	100	53.1	9748	PASS
70	69	0.00	2	0.6	55	PASS
127	198	10	80	53.0	9735	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18375	PASS
199	198	5	9	6.8	1255	PASS
275	198	10	60	27.6	5073	PASS
365	198	1	100	3.4	623	PASS
441	442	0.01	24	17.4	2233	PASS
442	198	50	100	69.9	12845	PASS
443	442	15	24	19.1	2450	PASS