


Data Path : Z:\HPCHEM1\BNA E\Data\BE022718\
 Data File : BE095696.D
 Acq On : 27 Feb 2018 10:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE022318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 23 12:12:42 2018

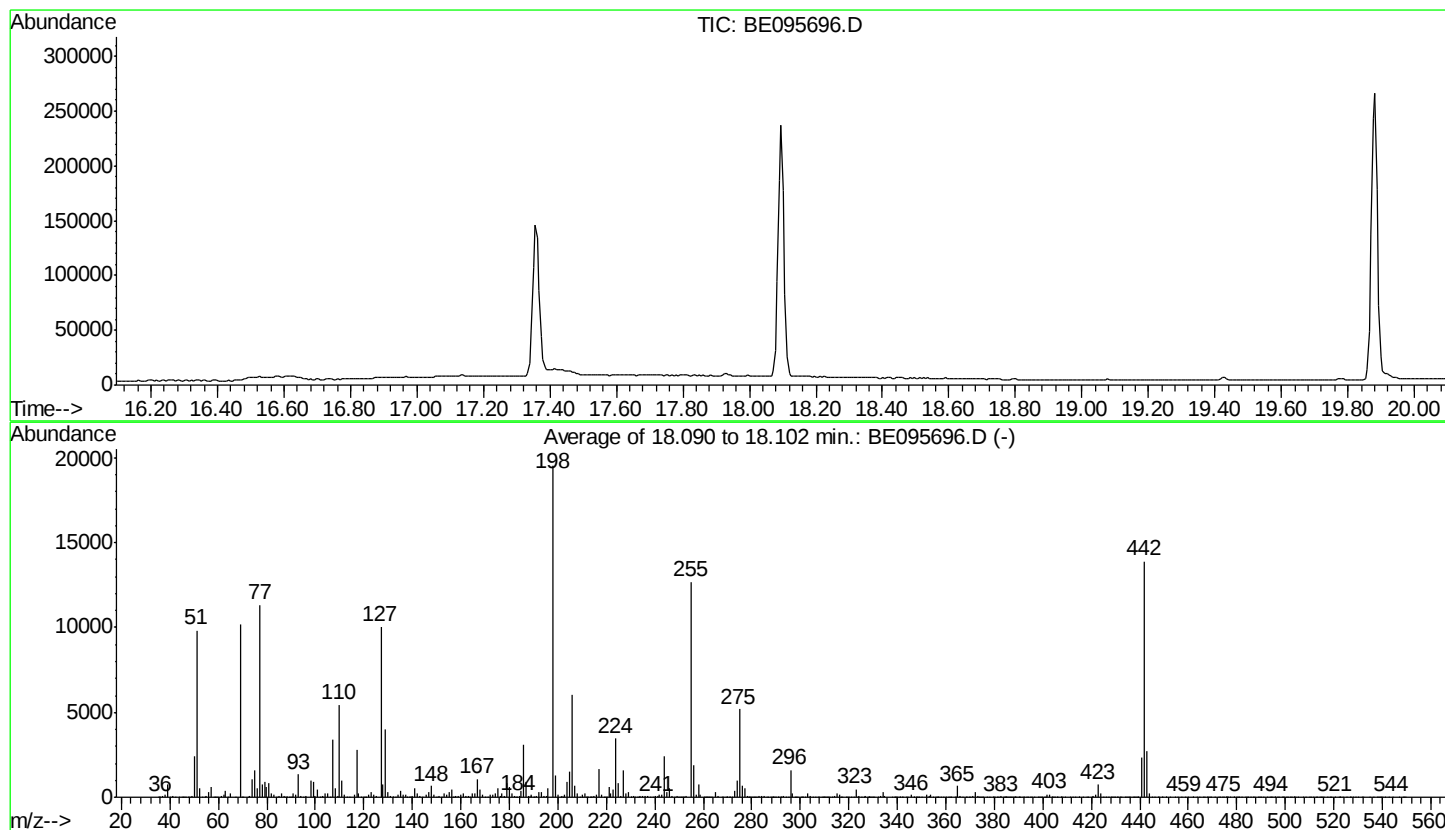

AutoFind: Scans 2638, 2639, 2640; Background Corrected with Scan 2630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.3	9826	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.0	10169	PASS
70	69	0.00	2	0.3	30	PASS
127	198	10	80	51.5	10068	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19544	PASS
199	198	5	9	6.7	1313	PASS
275	198	10	60	26.6	5190	PASS
365	198	1	100	3.3	651	PASS
441	442	0.01	24	16.7	2317	PASS
442	198	50	100	71.2	13908	PASS
443	442	15	24	19.3	2682	PASS