
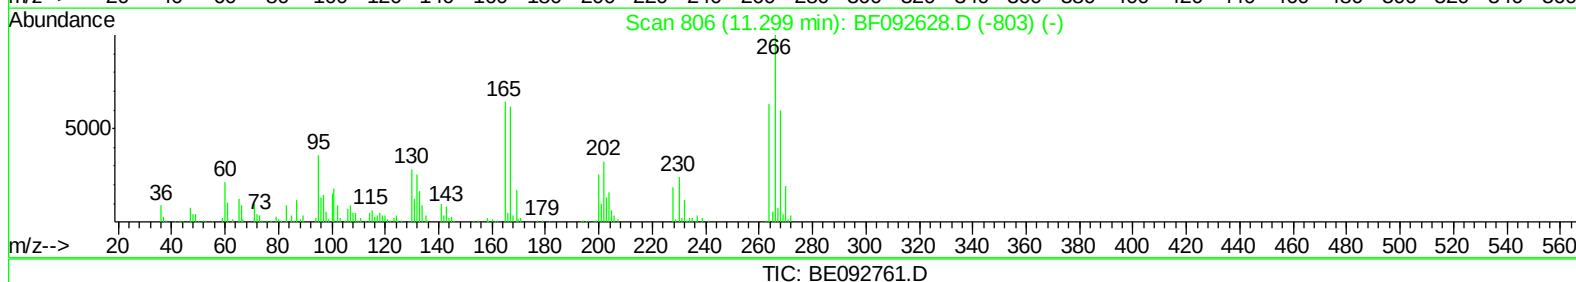
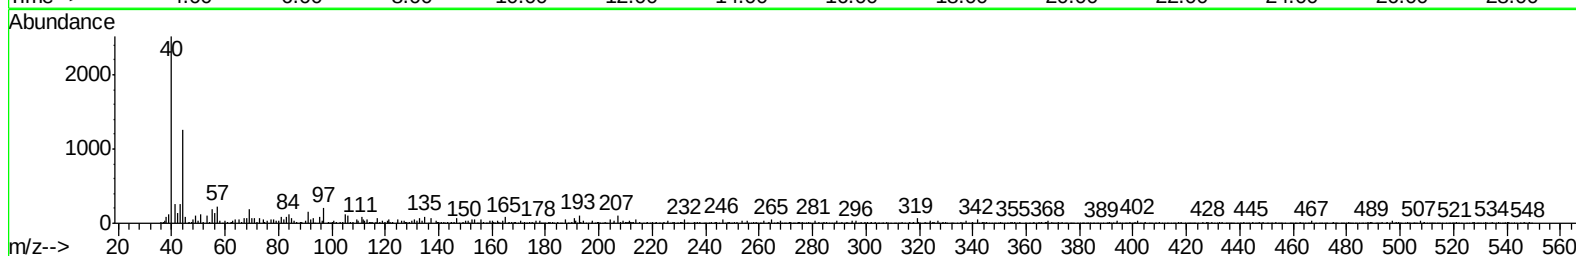


Data File : BE092761.D
Acq On : 28 Feb 2017 12:53
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 07:23:10 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

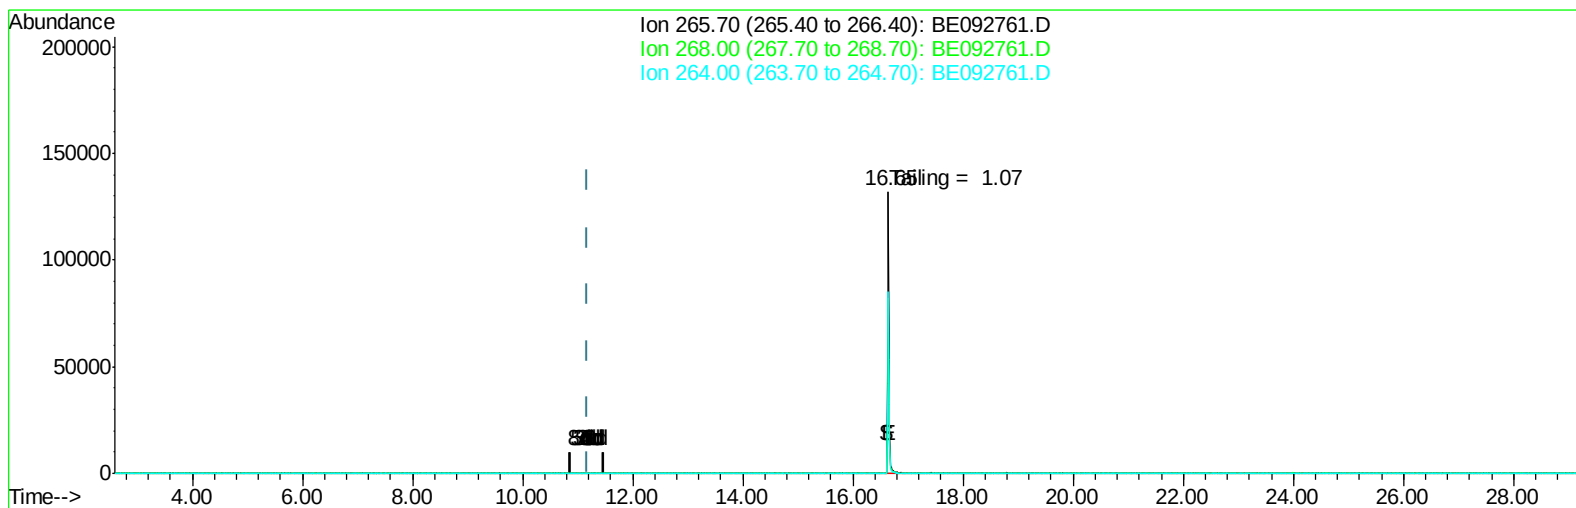




TIC: BE092761.D

(69) Pentachlorophenol (C)
11.184min (-0.001) 140.82ng
response 18

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	9.52#
264.00	62.90	2.38#
0.00	0.00	0.00

Data File : BE092761.D
Acq On : 28 Feb 2017 12:53
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 07:23:10 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

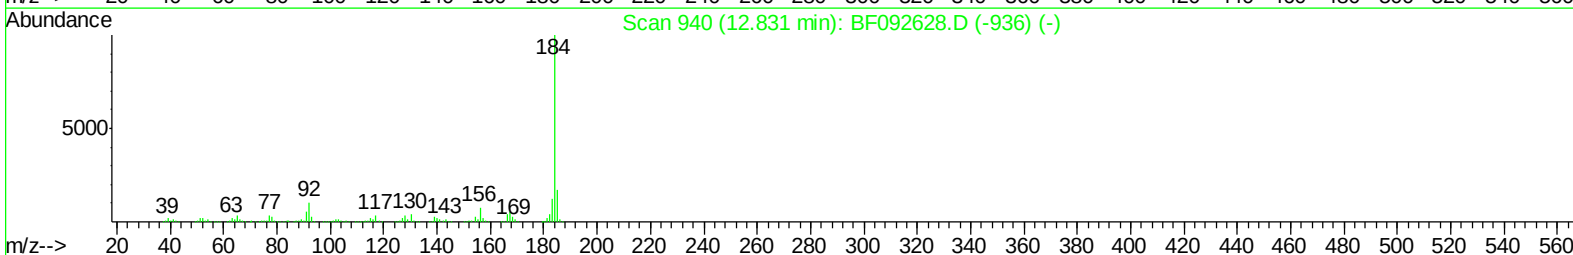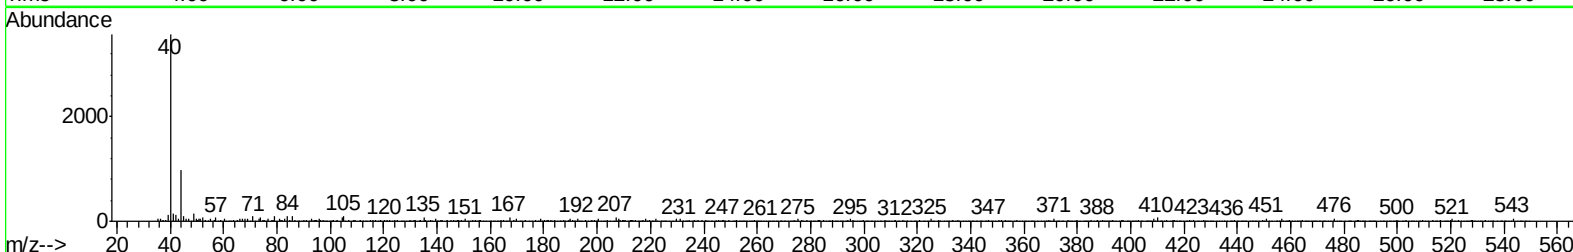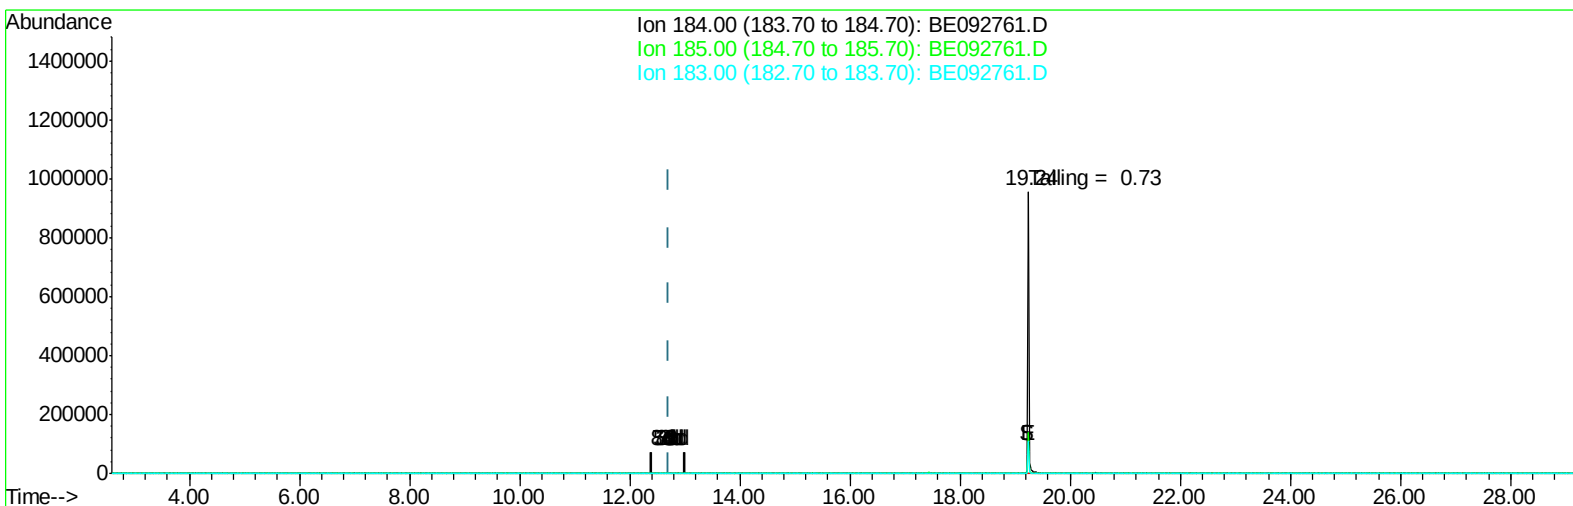

TIC: BE092761.D

(76) Benzidine

12.741min (+0.024) 28.57ng

response 28

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	3.85#
183.00	11.50	11.54
0.00	0.00	0.00