


Data Path : Z:\HPCHEM1\BNA E\DATA\BE022817\
 Data File : BE092761.D
 Acq On : 28 Feb 2017 12:53
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE021517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 15 17:05:20 2017

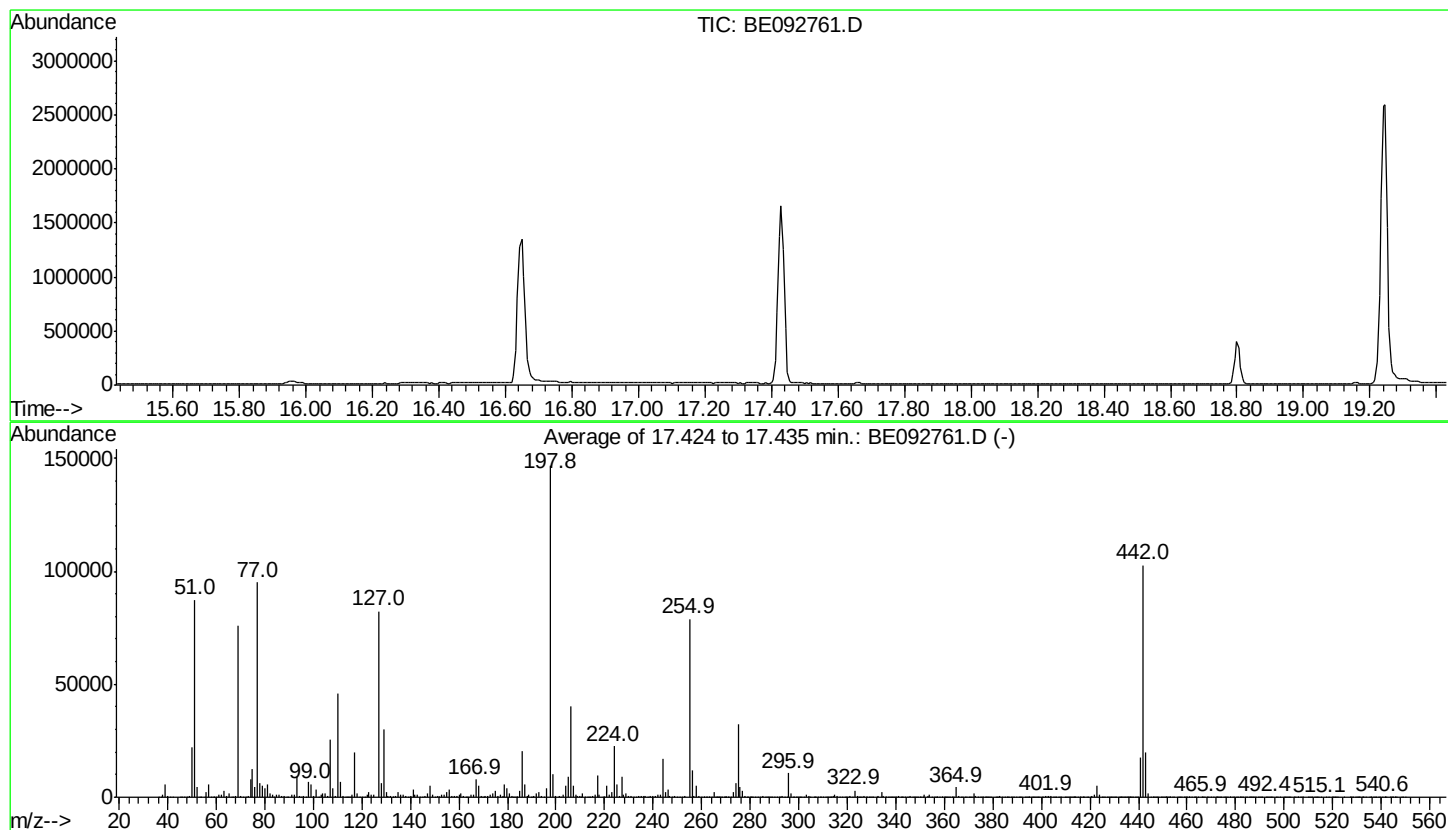

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.5	87334	PASS
68	69	0.00	2	1.0	732	PASS
69	198	0.00	100	51.8	76019	PASS
70	69	0.00	2	0.5	389	PASS
127	198	10	80	56.1	82304	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	146751	PASS
199	198	5	9	7.0	10335	PASS
275	198	10	60	22.0	32341	PASS
365	198	1	100	3.1	4527	PASS
441	442	0.01	24	17.0	17454	PASS
442	198	50	100	69.9	102589	PASS
443	442	15	24	19.5	19975	PASS