


Data Path : Z:\HPCHEM1\BNA E\DATA\BE030117\
 Data File : BE092775.D
 Acq On : 1 Mar 2017 9:32
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE021517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 15 17:05:20 2017

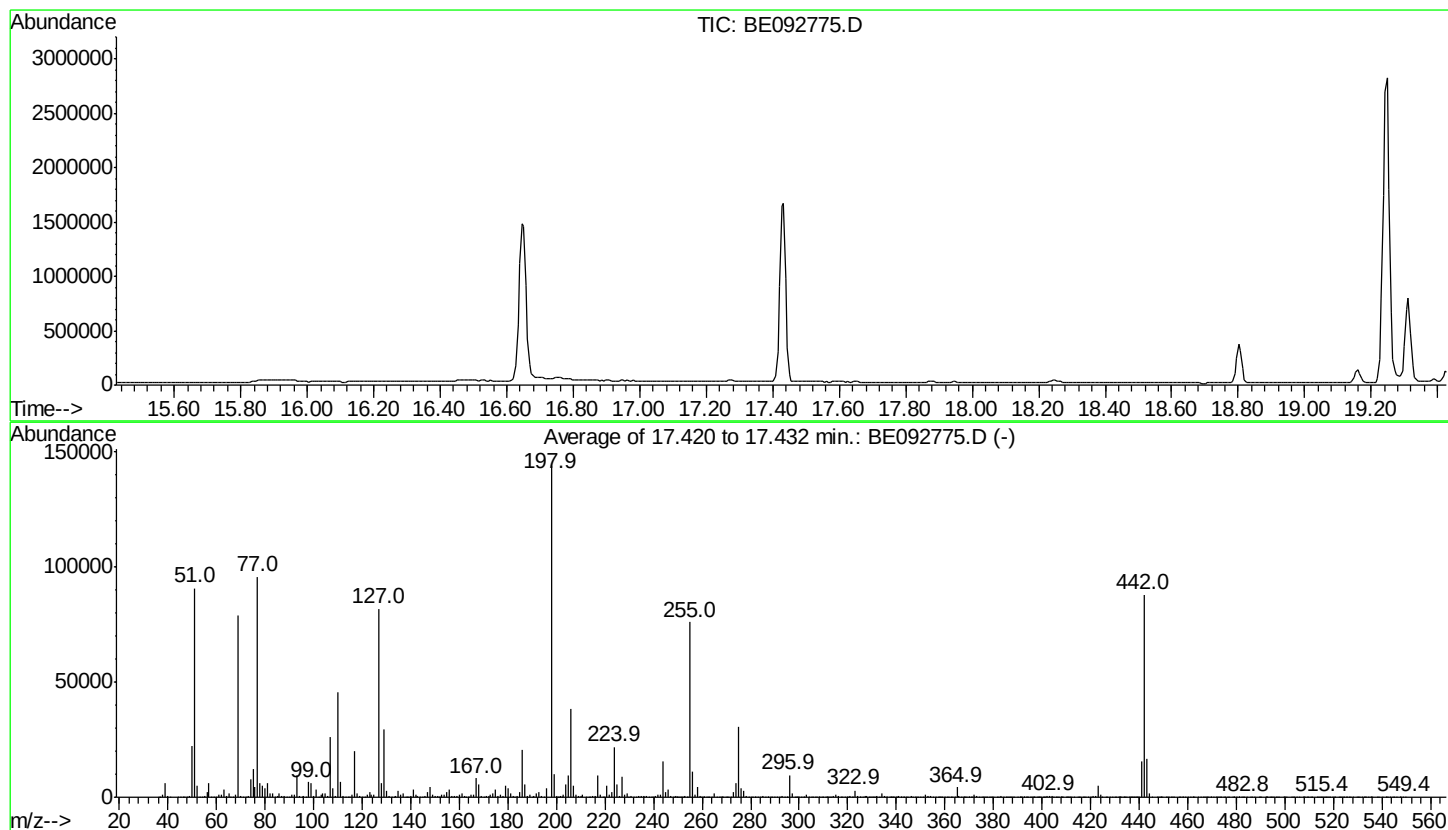

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.0	90654	PASS
68	69	0.00	2	1.6	1271	PASS
69	198	0.00	100	54.7	78680	PASS
70	69	0.00	2	0.6	465	PASS
127	198	10	80	56.8	81794	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	143897	PASS
199	198	5	9	6.8	9820	PASS
275	198	10	60	21.1	30349	PASS
365	198	1	100	3.0	4318	PASS
441	442	0.01	24	17.8	15638	PASS
442	198	50	100	61.2	88026	PASS
443	442	15	24	19.3	16950	PASS