


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE030315\
 Data File : BE089722.D
 Acq On : 3 Mar 2015 10:03
 Operator : TP/JJ
 Sample : DFTPP01
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP01

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE030315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 04 04:20:28 2015

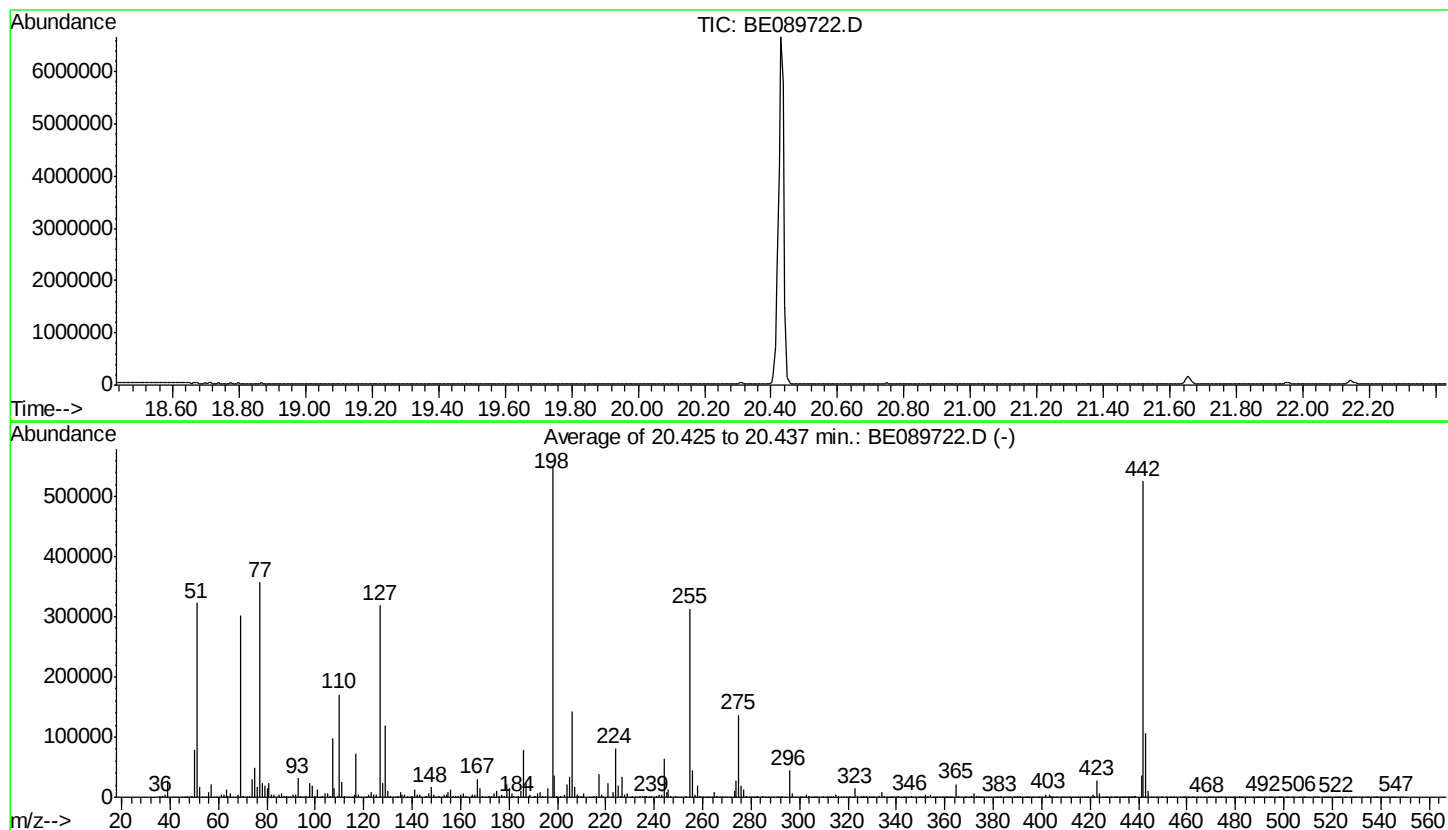

AutoFind: Scans 3240, 3241, 3242; Background Corrected with Scan 3230

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.6	322944	PASS
68	69	0.00	2	1.6	4862	PASS
69	198	0.00	100	54.7	301717	PASS
70	69	0.00	2	0.5	1572	PASS
127	198	10	80	57.7	318314	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	551360	PASS
199	198	5	9	6.8	37341	PASS
275	198	10	60	24.8	136901	PASS
365	198	1	100	3.9	21772	PASS
441	443	0.01	100	34.0	35986	PASS
442	198	50	100	95.2	524885	PASS
443	442	15	24	20.2	105813	PASS