


Data Path : Z:\HPCHEM1\BNA_E\Data\BE030316\
Data File : BE091422.D
Acq On : 3 Mar 2016 14:45
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE030316.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 04 11:58:27 2016

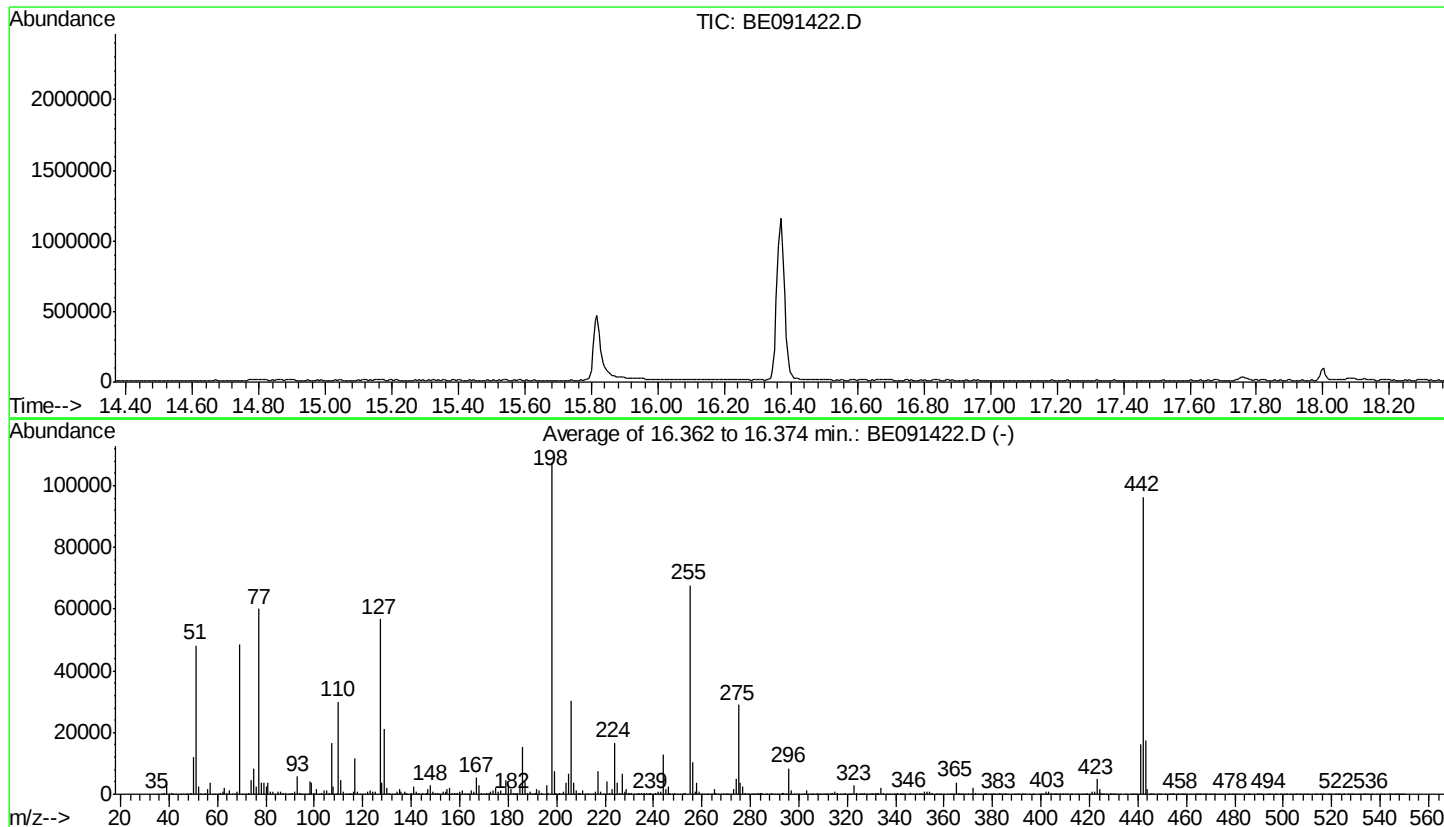

AutoFind: Scans 2344, 2345, 2346; Background Corrected with Scan 2332

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	48232	PASS
68	69	0.00	2	1.4	685	PASS
69	198	0.00	100	45.1	48453	PASS
70	69	0.00	2	0.4	176	PASS
127	198	10	80	52.7	56675	PASS
197	198	0.00	2	0.3	298	PASS
198	198	100	100	100.0	107483	PASS
199	198	5	9	7.0	7541	PASS
275	198	10	60	26.9	28860	PASS
365	198	1	100	3.6	3896	PASS
441	442	0.01	24	16.9	16330	PASS
442	198	50	100	89.7	96436	PASS
443	442	15	24	18.1	17423	PASS