


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE030415\
 Data File : BE089728.D
 Acq On : 4 Mar 2015 16:41
 Operator : TP/JJ
 Sample : DFTPP02
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE030315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 05 00:14:14 2015

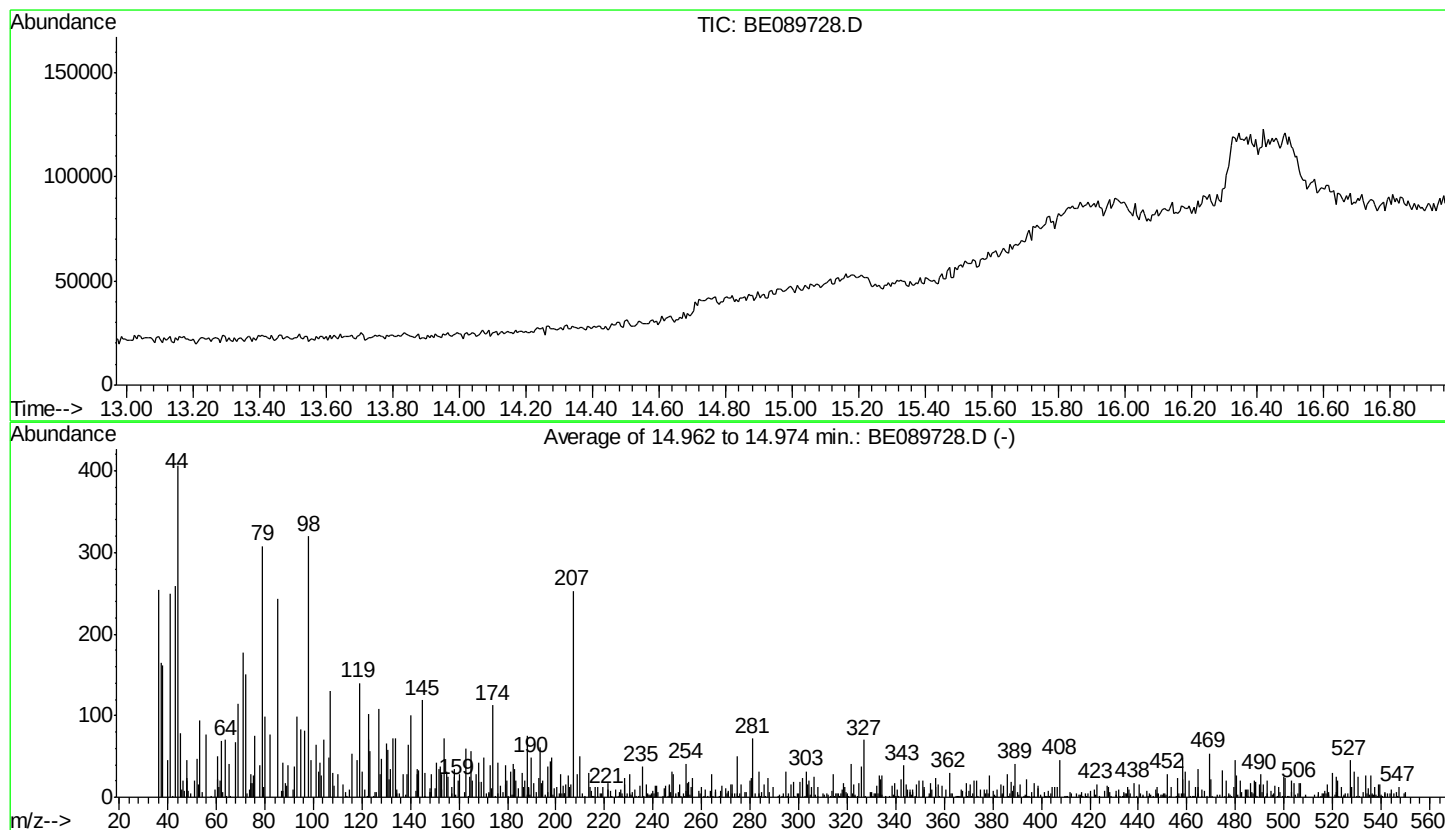

AutoFind: Scans 2310, 2311, 2312; Background Corrected with Scan 2308

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	21	PASS
68	69	0.00	2	58.3	67	FAIL*
69	198	0.00	100	234.7	115	FAIL*
70	69	0.00	2	0.0	0	PASS
127	198	10	80	220.4	108	FAIL*
197	198	0.00	1	12.2	6	FAIL*
198	198	100	100	100.0	49	PASS
199	198	5	9	22.4	11	FAIL*
275	198	10	60	104.1	51	FAIL*
365	198	1	100	4.1	2	PASS
441	443	0.01	100	62.5	5	PASS
442	198	50	100	6.1	3	FAIL*
443	442	15	24	266.7	8	FAIL*