

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE030515\
 Data File : BE089748.D
 Acq On : 5 Mar 2015 17:31
 Operator : TP/JJ
 Sample : MDL-06-S
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Mar 06 09:53:00 2015

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE030315.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Mar 04 14:17:55 2015


Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	9.33	152	4603	0.40	ng/ul	0.00
4) Naphthalene-d8	12.23	136	19364	0.40	ng/ul	0.00
8) Acenaphthene-d10	16.40	164	8353	0.40	ng/ul	0.00
12) Phenanthrene-d10	19.76	188	14490	0.40	ng/ul	0.00
18) Chrysene-d12	23.65	240	7562	0.40	ng/ul	0.00
22) Perylene-d12	25.33	264	3024	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.63	96	11583	1.91	ng/uL	0.00
6) 2-Methylnaphthalene-d10	0.00	152	0d	0.00	ng/ul	
16) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
3) 1,4-Dioxane	2.70	88	2807	0.40	ng/ul#	Qvalue 83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE030515\
Data File : BE089748.D
Acq On : 5 Mar 2015 17:31
Operator : TP/JJ
Sample : MDL-06-S
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Mar 06 09:53:00 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE030315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 14:17:55 2015
Response via : Initial Calibration

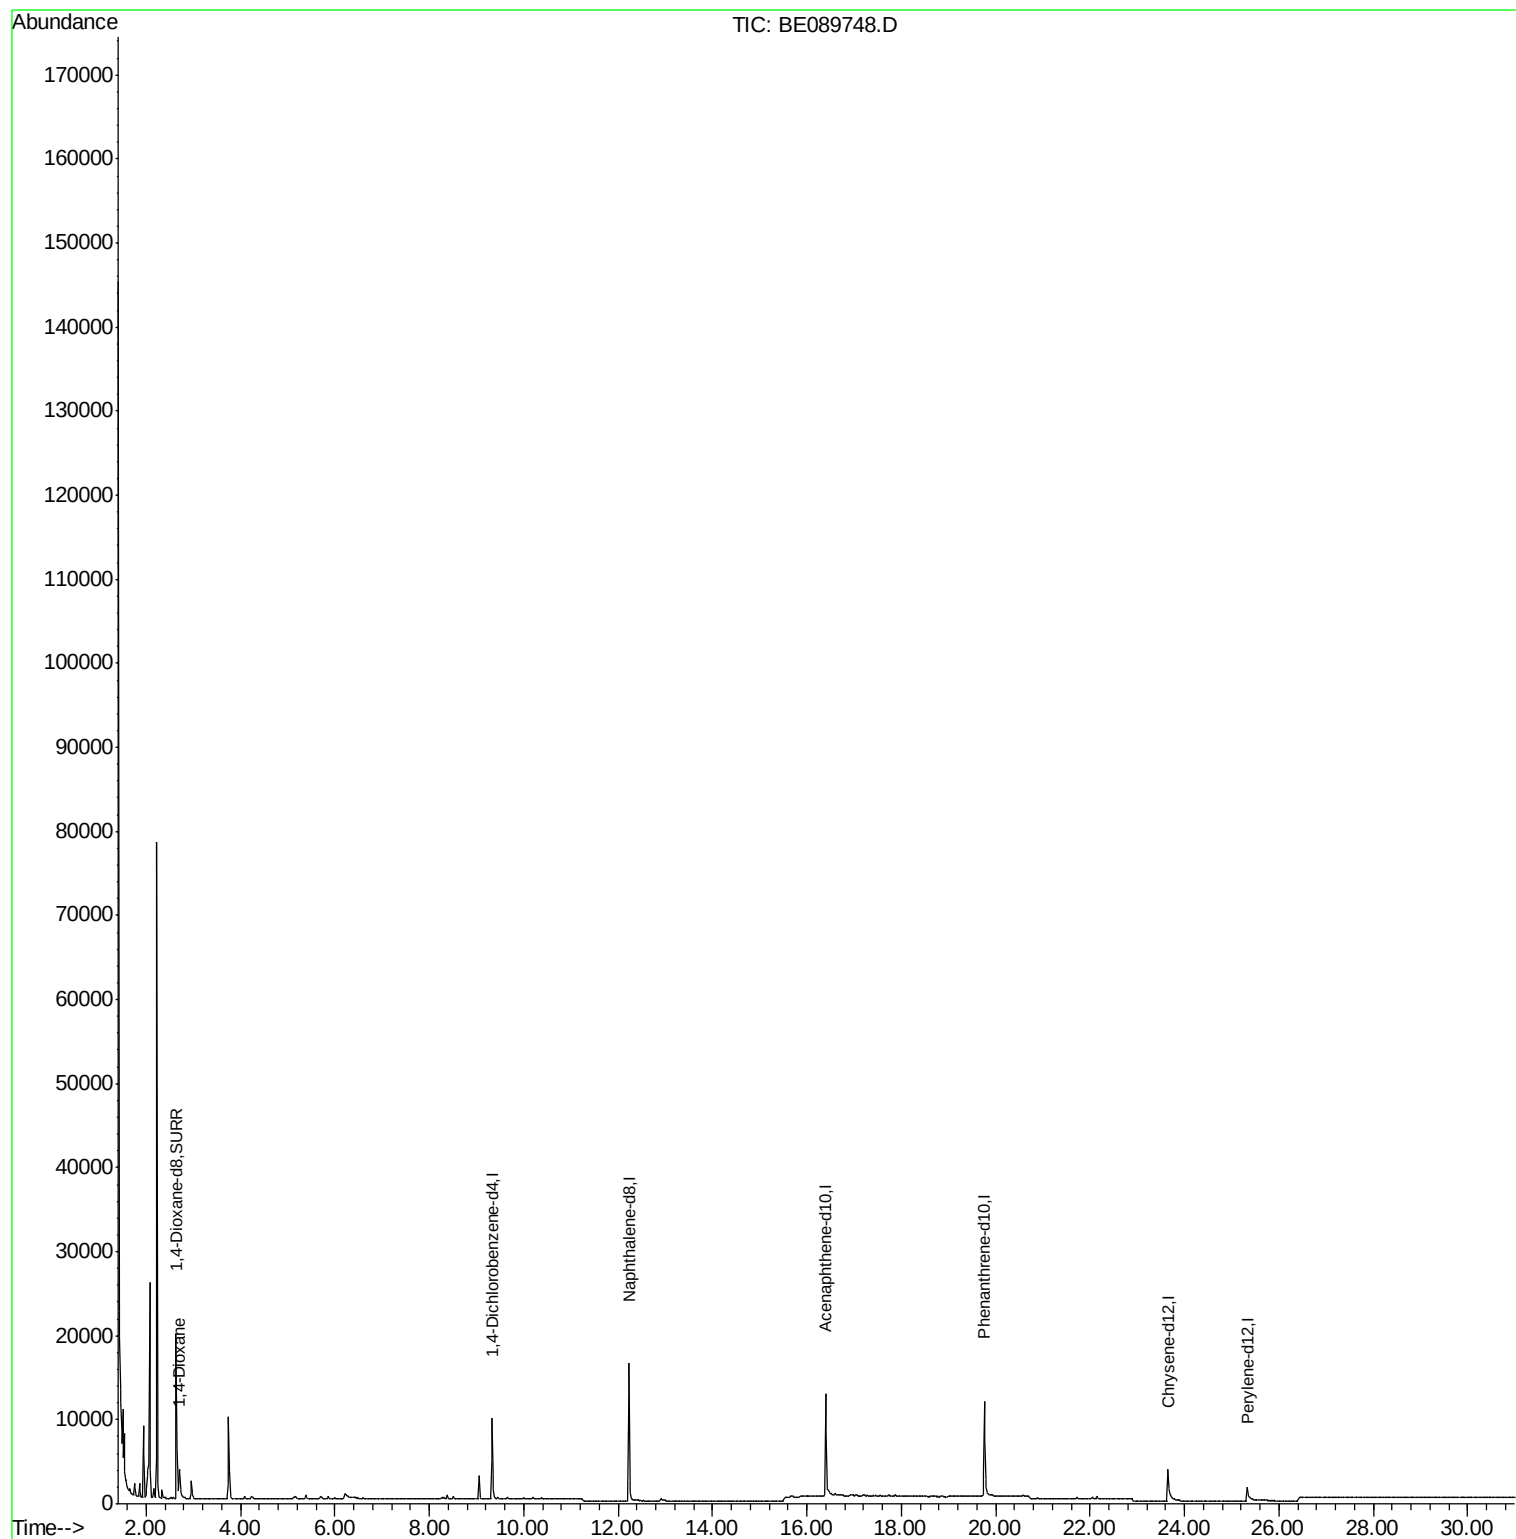

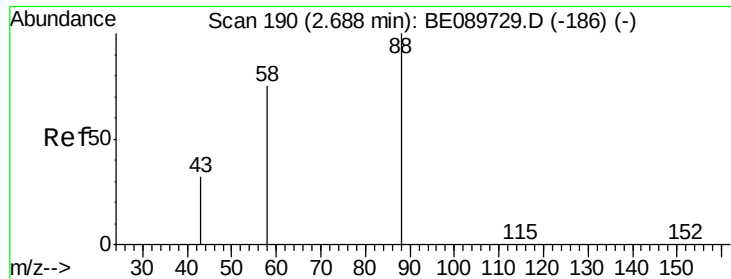

#3

1,4-Dioxane

Concen: 0.40 ng/ul

RT: 2.70 min Scan# 192

Delta R.T. 0.02 min

Lab File: BE089748.D

Acq: 5 Mar 2015 17:31

Tgt Ion: 88 Resp: 2807

Ion Ratio Lower Upper

88 100

58 76.7 61.3 91.9

43 0.0 26.1 39.1#

