


Data Path : Z:\HPCHEM1\BNA_E\Data\BE030515\
 Data File : BE089740.D
 Acq On : 5 Mar 2015 12:02
 Operator : TP/JJ
 Sample : DFTPP03
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE030315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 04 14:17:55 2015

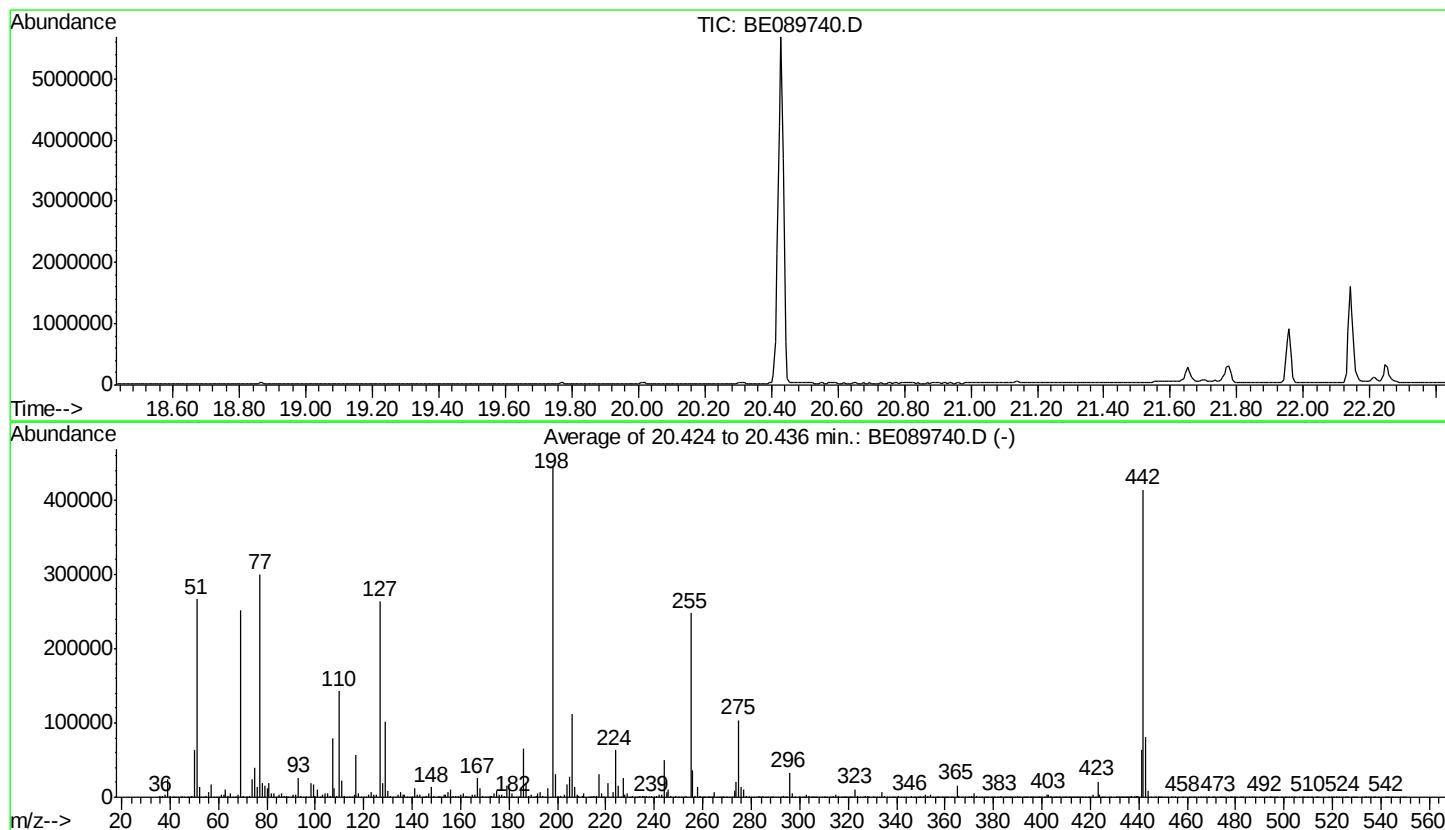

AutoFind: Scans 3240, 3241, 3242; Background Corrected with Scan 3229

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.8	266935	PASS
68	69	0.00	2	1.3	3277	PASS
69	198	0.00	100	56.5	252135	PASS
70	69	0.00	2	0.6	1478	PASS
127	198	10	80	59.0	263168	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	446139	PASS
199	198	5	9	6.9	30818	PASS
275	198	10	60	23.3	104103	PASS
365	198	1	100	3.6	16030	PASS
441	443	0.01	100	77.8	62958	PASS
442	198	50	100	92.8	414068	PASS
443	442	15	24	19.6	80953	PASS