
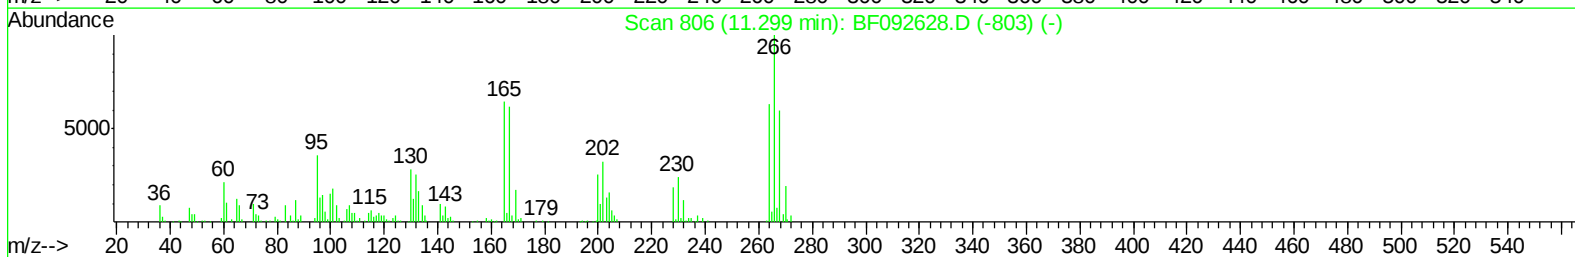
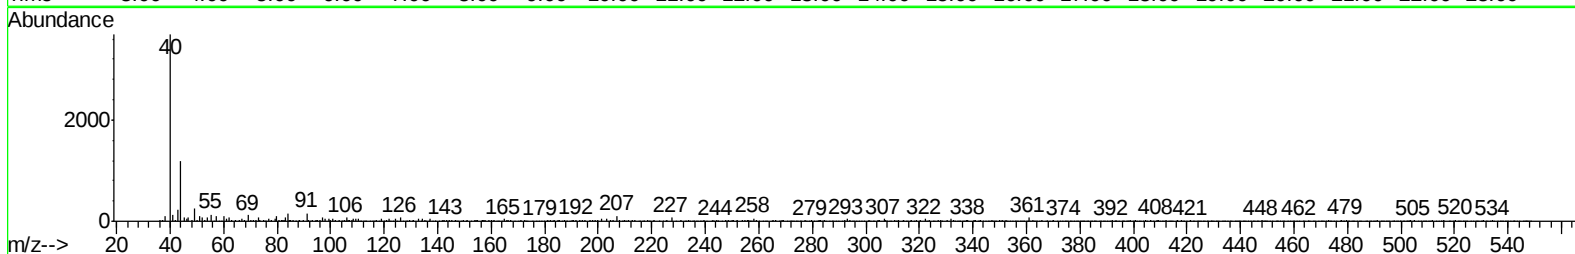


Data Path : Z:\HPCHEM1\BNA_E\Data\BE030617\
Data File : BE092779.D
Acq On : 6 Mar 2017 9:37
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 06:30:07 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

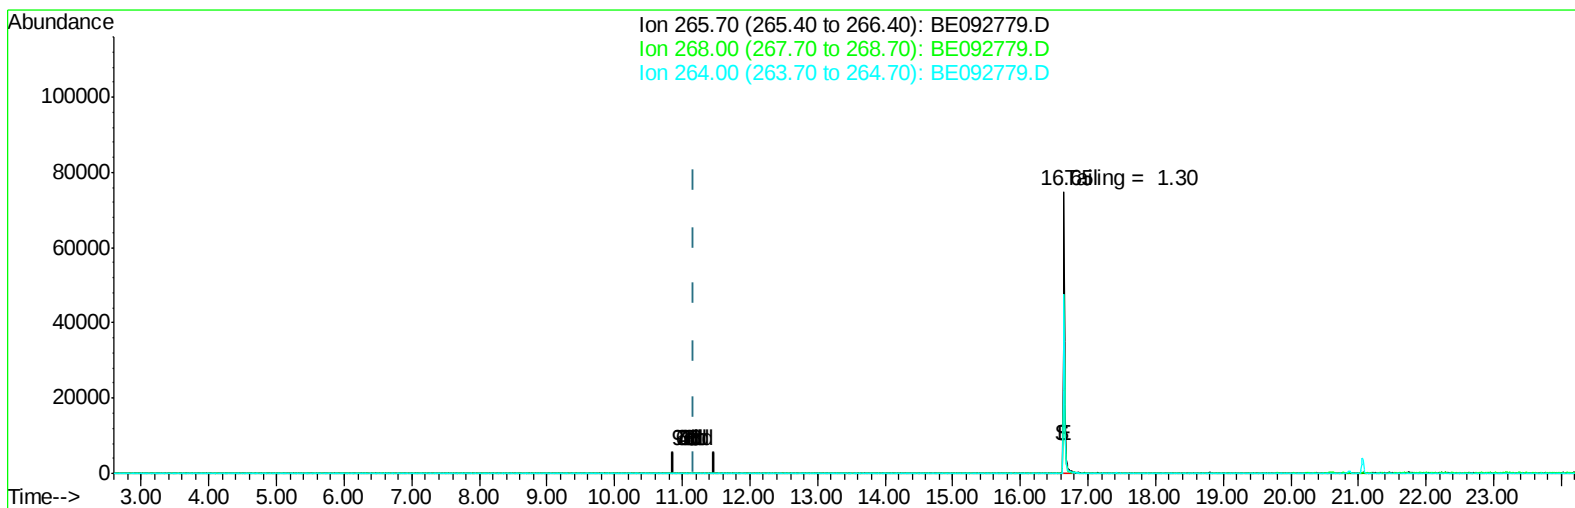

TIC: BE092779.D

(69) Pentachlorophenol (C)




11.171min (-0.014) 117.47ng

response 31

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	60.00
264.00	62.90	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE030617\
Data File : BE092779.D
Acq On : 6 Mar 2017 9:37
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 06:30:07 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

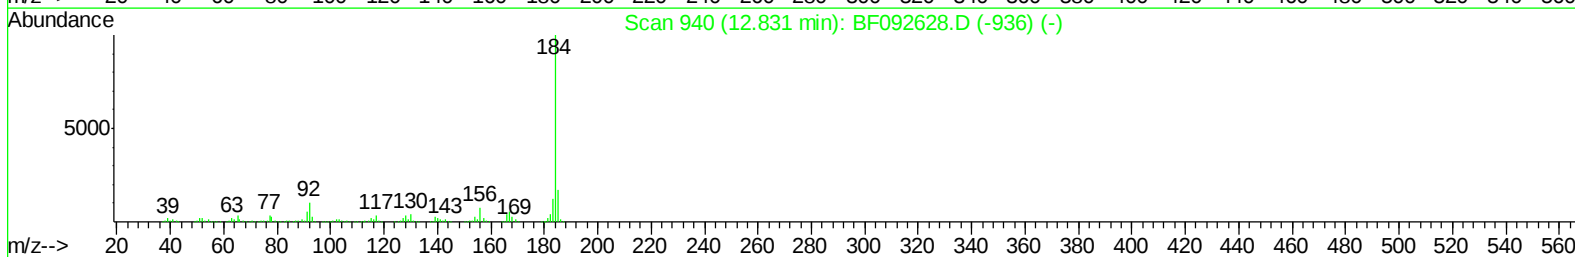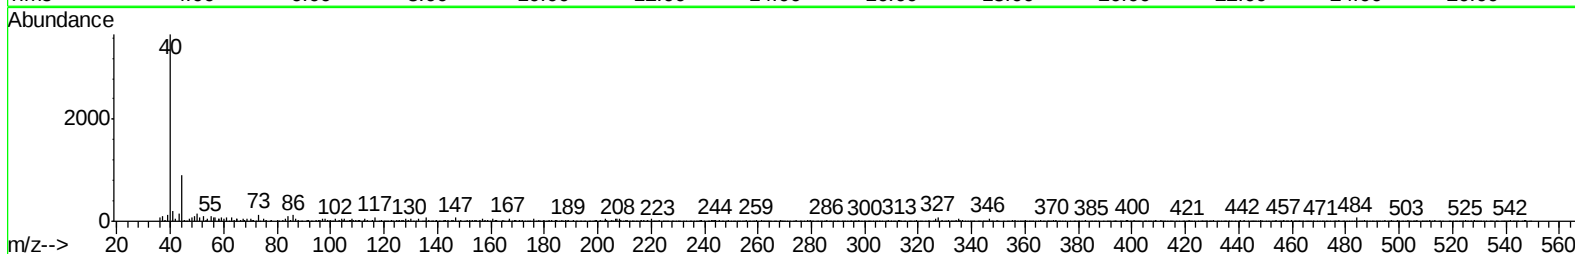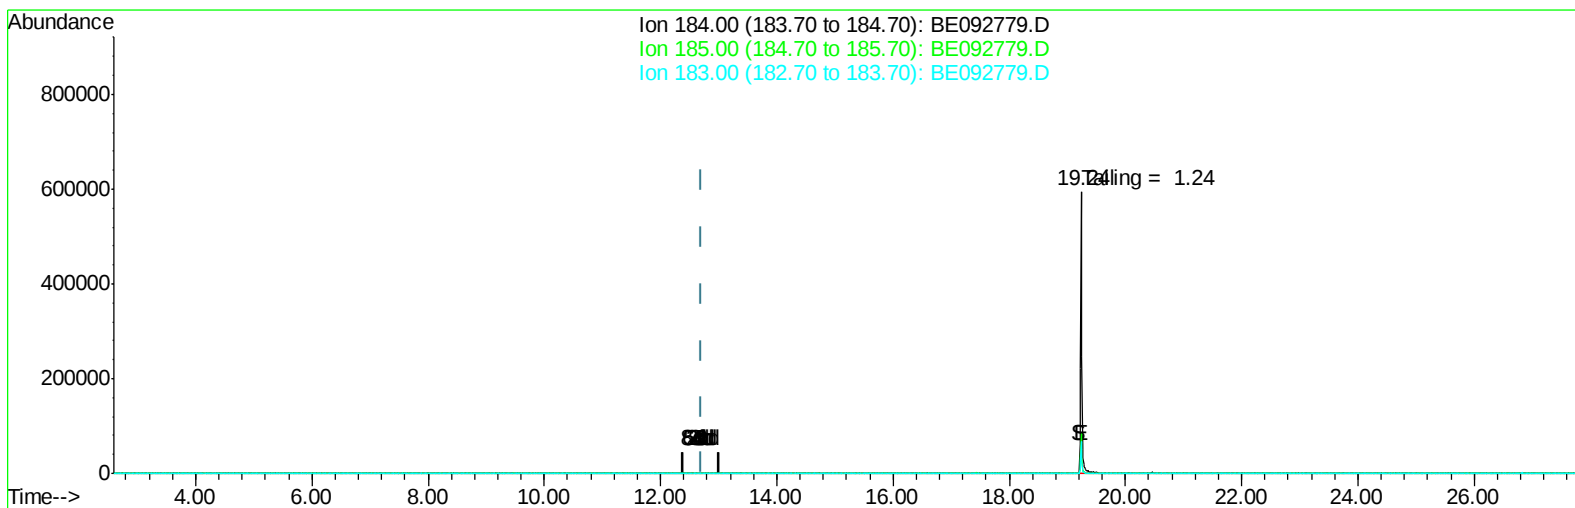

TIC: BE092779.D

(76) Benzidine

12.693min (-0.024) 62.58ng

response 32

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.22
183.00	11.50	41.30#
0.00	0.00	0.00