

Data Path : Z:\HPCHEM1\BNA E\DATA\BE030617\
 Data File : BE092785.D
 Acq On : 6 Mar 2017 13:24
 Operator : SJ/MA
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Manual Integrations
 APPROVED

mohammad
 3/7/2017 4:22:46 PM


Quant Time: Mar 06 14:36:48 2017
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE030617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 06 14:29:53 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	9783	5.00	ng	0.00
7) Naphthalene-d8	10.87	136	43694	5.00	ng	0.00
12) Acenaphthene-d10	14.75	164	28018	5.00	ng	0.00
18) Phenanthrene-d10	17.51	188	52162	5.00	ng	0.00
24) Chrysene-d12	21.68	240	81522	5.00	ng	0.00
31) Perylene-d12	24.01	264	71870	5.00	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.60	112	6668	3.50	ng	0.00
5) Phenol-d6	7.27	99	8890	3.81	ng	-0.02
8) Nitrobenzene-d5	9.27	82	8989	3.69	ng	-0.02
13) 2,4,6-Tribromophenol	16.25	330	2491	4.19	ng	-0.01
14) 2-Fluorobiphenyl	13.36	172	21149	3.10	ng	-0.02
26) Terphenyl-d14	20.11	244	28422	2.73	ng	-0.02

Target Compounds				Qvalue		
2) 1,4-Dioxane	3.33	88	3779	2.72	ng	95
3) n-Nitrosodimethylamine	3.68	42	5378	3.71	ng	98
6) bis(2-Chloroethyl)ether	7.52	93	8935	3.46	ng	# 28
9) Naphthalene	10.91	128	29499	3.12	ng	# 95
10) Hexachlorobutadiene	11.20	225	4193	3.02	ng	100
11) 2-Methylnaphthalene	12.55	142	19447	3.27	ng	# 87
15) Acenaphthylene	14.46	152	134614	3.18	ng	100
16) Acenaphthene	14.82	154	19547	3.18	ng	91
17) Fluorene	15.80	166	25656	3.25	ng	99
19) Hexachlorobenzene	16.82	284	7308	3.63	ng	# 66
20) Pentachlorophenol	17.17	266	2509	5.67	ng	# 84
21) Phenanthrene	17.53	178	42864	3.46	ng	# 94
22) Anthracene	17.63	178	43354	3.80	ng	98
23) Fluoranthene	19.54	202	203076	3.82	ng	98
25) Pyrene	19.90	202	224540	2.89	ng	100
27) Benzo(a)anthracene	21.66	228	254302m	3.22	ng	
28) Chrysene	21.70	228	231825m	2.47	ng	
29) Bis(2-ethylhexyl)phthalate	21.59	149	19263	1.75	ng	# 72
30) Indeno(1,2,3-cd)pyrene	26.45	276	264484	2.50	ng	97
32) Benzo(b)fluoranthene	23.28	252	63780	3.14	ng	94
33) Benzo(k)fluoranthene	23.34	252	56957	2.65	ng	95
34) Benzo(a)pyrene	23.89	252	57848	3.13	ng	94
35) Dibenzo(a,h)anthracene	26.46	278	55770	2.86	ng	95
36) Benzo(g,h,i)perylene	27.20	276	231682	2.81	ng	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 8.10 min Scan# 573

Delta R.T. 0.00 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Instrument :

BNA_E





ClientSampleId :

SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.1	106.0	159.0
115	52.7	31.2	46.8

Manual Integrations
APPROVED

mohammad
3/7/2017 4:22:46 PM



#2

1,4-Dioxane

Concen: 2.72 ng




RT: 3.33 min Scan# 64




Delta R.T. 0.00 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Lower	Upper
88	100		
58	85.1	63.6	95.4
43	36.7	28.0	42.0





#3

n-Nitrosodimethylamine

Concen: 3.71 ng

RT: 3.68 min Scan# 94

Delta R.T. -0.02 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Tot Ion:	42	Resp:	5378
Ion	Ratio	Lower	Upper
42	100		
74	105.7	86.0	129.0
44	6.7	5.1	7.7

Instrument :





BNA_E

ClientSampleId :

SSTDICC3.2

Manual Integrations
APPROVED

mohammad
3/7/2017 4:22:46 PM



#4

2-Fluorophenol

Concen: 3.50 ng


RT: 5.60 min Scan# 351


Delta R.T. -0.01 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Tgt Ion:	112	Resp:	6668
Ion	Ratio	Lower	Upper
112	100		
64	68.0	53.5	80.3
63	36.7	27.9	41.9

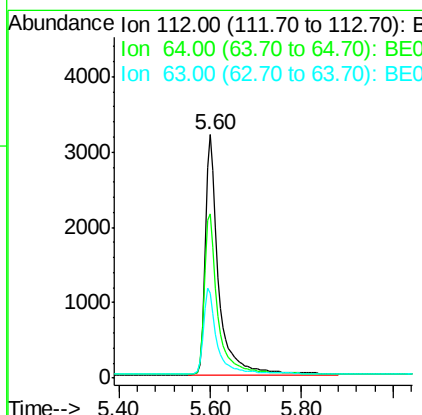



#5

Phenol-d6

Concen: 3.81 ng

RT: 7.27 min Scan# 537

Delta R.T. -0.02 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Instrument :

BNA_E


ClientSampleId :

SSTDICC3.2




Tot Ion:	99	Resp:	8890
Ion	Ratio	Lower	Upper
99	100		
42	24.2	16.0	24.0#
71	32.8	30.6	45.8

Manual Integrations
APPROVED

mohammad
3/7/2017 4:22:46 PM



Abundance Ion 99.00 (98.70 to 99.70): BE0
Ion 42.00 (41.70 to 42.70): BE0
Ion 71.00 (70.70 to 71.70): BE0

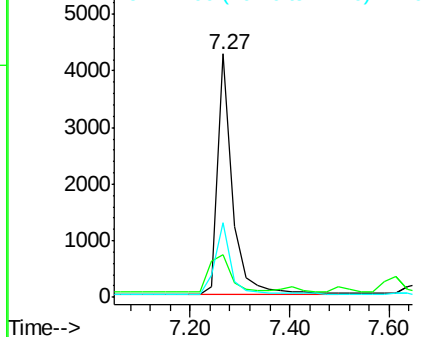

#6

bis(2-Chloroethyl)ether

Concen: 3.46 ng


RT: 7.52 min Scan# 548

Delta R.T. 0.00 min



Lab File: BE092785.D


Acq: 6 Mar 2017 13:24

Tgt Ion:	93	Resp:	8935
Ion	Ratio	Lower	Upper
93	100		
63	0.0	71.6	107.4#
95	31.6	24.0	36.0



Abundance Ion 93.00 (92.70 to 93.70): BE0
Ion 63.00 (62.70 to 63.70): BE0
Ion 95.00 (94.70 to 95.70): BE0

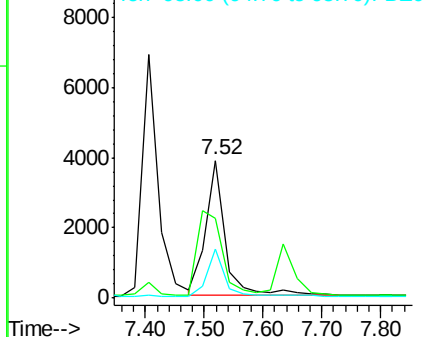



#7

Naphthalene-d8

Concen: 5.00 ng

RT: 10.87 min Scan# 704

Delta R.T. -0.00 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Instrument :

BNA_E


ClientSampleId :

SSTDICC3.2

Tot Ion	Ratio	Resp	Lower	Upper
136	100	43694		
137	11.5		8.2	12.4
54	6.4		9.6	14.4#
68	4.9		6.7	10.1#

Manual Integrations
APPROVED

mohammad
3/7/2017 4:22:46 PM






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

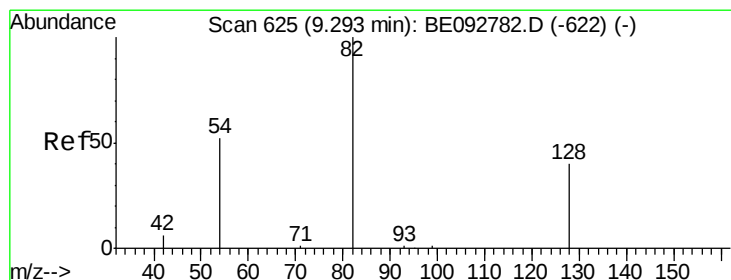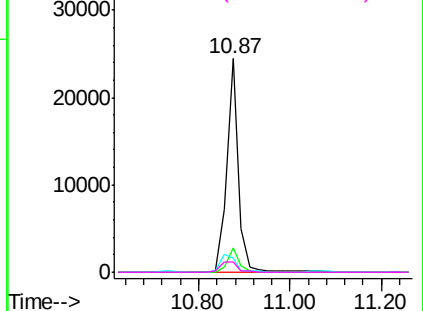

#8

Nitrobenzene-d5

Concen: 3.69 ng


RT: 9.27 min Scan# 624

Delta R.T. -0.02 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24



Tgt Ion	Ratio	Resp	Lower	Upper
82	100	8989		
128	49.2		39.0	58.4
54	41.8		44.8	67.2#




Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

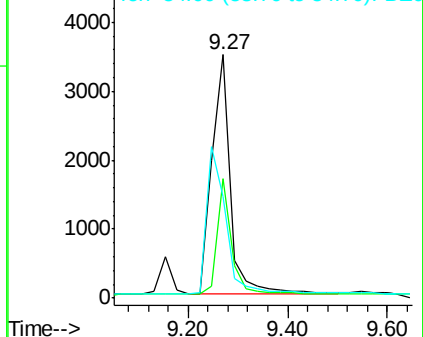



#9

Naphthalene

Concen: 3.12 ng

RT: 10.91 min Scan# 706

Delta R.T. -0.02 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Instrument :

BNA_E





ClientSampleId :

SSTDICC3.2

Tot Ion:	128	Resp:	29499
Ion Ratio	Lower	Upper	
128	100		
129	10.3	11.2	16.8#
127	14.1	11.6	17.4

Manual Integrations
APPROVED

mohammad
3/7/2017 4:22:46 PM



#10

Hexachlorobutadiene

Concen: 3.02 ng




RT: 11.20 min Scan# 721


Delta R.T. -0.00 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Tgt Ion:	225	Resp:	4193
Ion Ratio	Lower	Upper	
225	100		
223	64.1	50.6	76.0
227	64.2	51.4	77.0



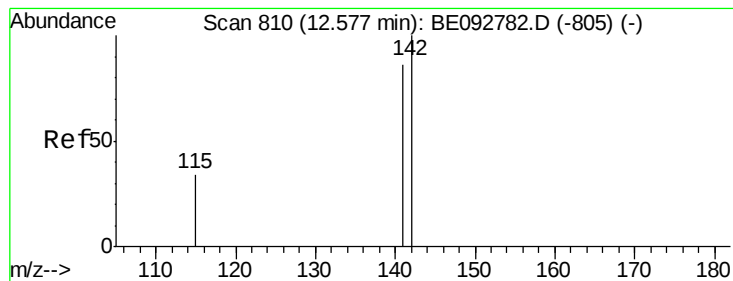





#11
2-Methylnaphthalene
Concen: 3.27 ng
RT: 12.55 min Scan# 808
Delta R.T. -0.02 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Instrument :
BNA_E
ClientSampled :
SSTDICC3.2

Tot Ion:142 Resp: 19447
Ion Ratio Lower Upper
142 100
141 82.4 73.7 110.5
115 31.2 34.0 51.0#




Manual Integrations
APPROVED


mohammad
3/7/2017 4:22:46 PM

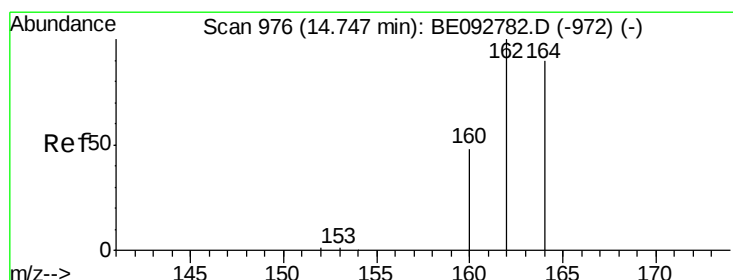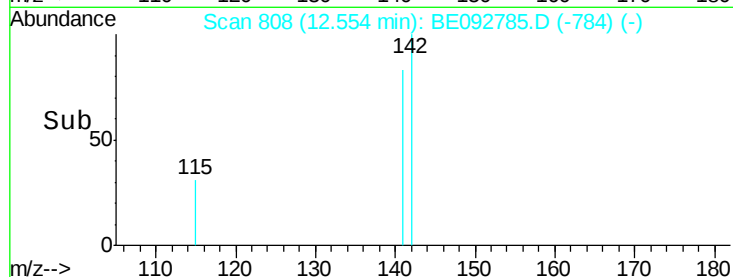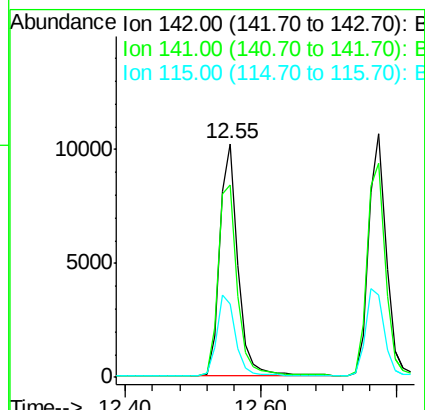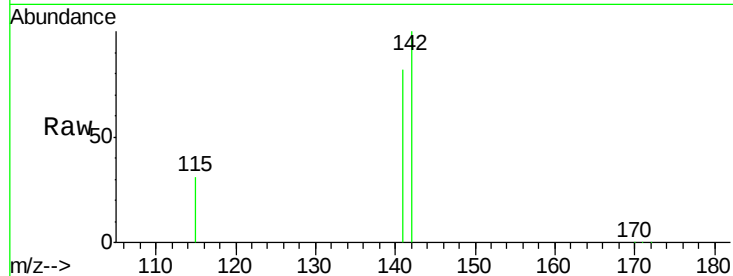

#12
Acenaphthene-d10
Concen: 5.00 ng
RT: 14.75 min Scan# 976
Delta R.T. 0.00 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Tgt Ion:164 Resp: 28018
Ion Ratio Lower Upper
164 100
162 103.5 71.4 107.0
160 45.5 27.4 41.2#

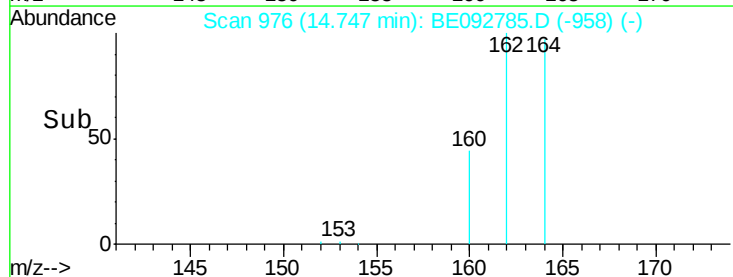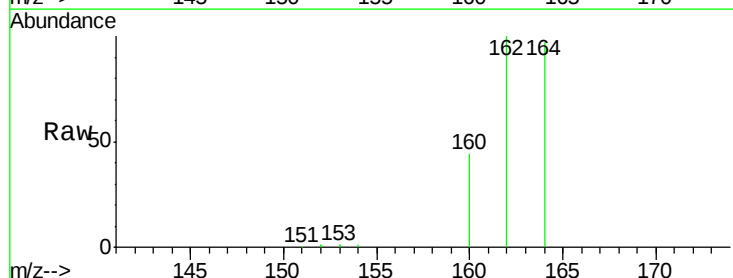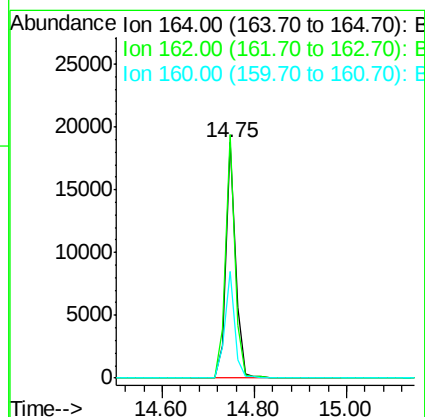

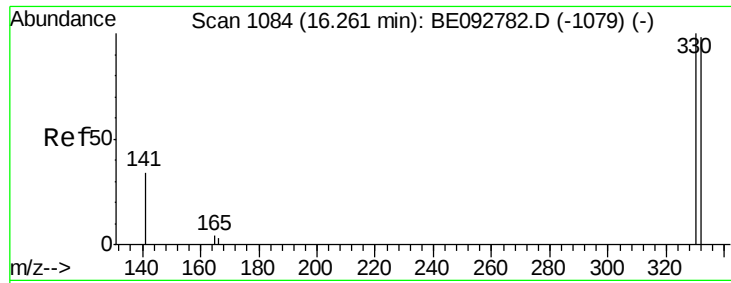





#13
 2,4,6-Tribromophenol
 Concen: 4.19 ng
 RT: 16.25 min Scan# 1083
 Delta R.T. -0.01 min
 Lab File: BE092785.D
 Acq: 6 Mar 2017 13:24

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.4	75.4	113.0
141	41.8	31.0	46.6




Manual Integrations
 APPROVED


mohammad
 3/7/2017 4:22:46 PM

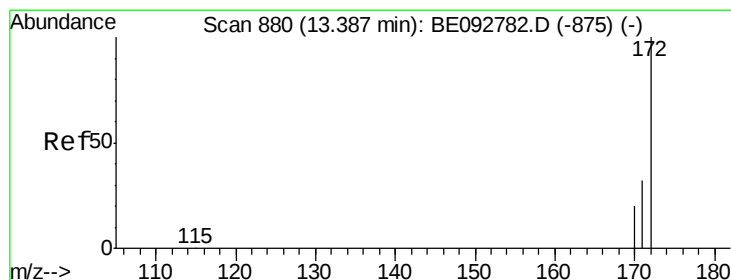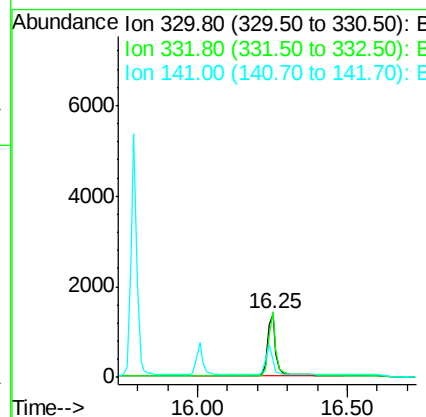

#14
 2-Fluorobiphenyl
 Concen: 3.10 ng
 RT: 13.36 min Scan# 878
 Delta R.T. -0.02 min
 Lab File: BE092785.D
 Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.1	30.1	45.1
170	23.8	21.8	32.6

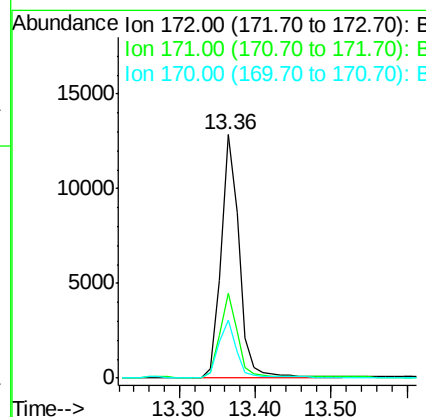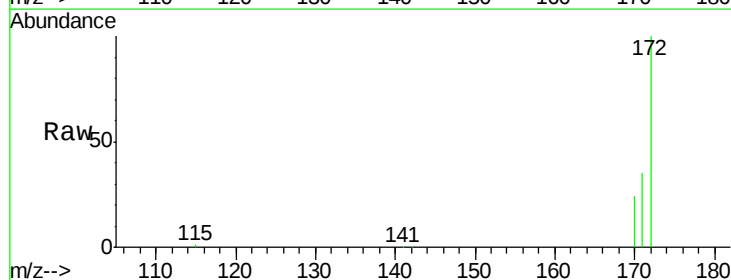







#15
Acenaphthylene
Concen: 3.18 ng
RT: 14.46 min Scan# 959
Delta R.T. 0.00 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
152	100		
151	4.9	3.9	5.9
153	13.0	10.4	15.6




Manual Integrations
APPROVED


mohammad
3/7/2017 4:22:46 PM

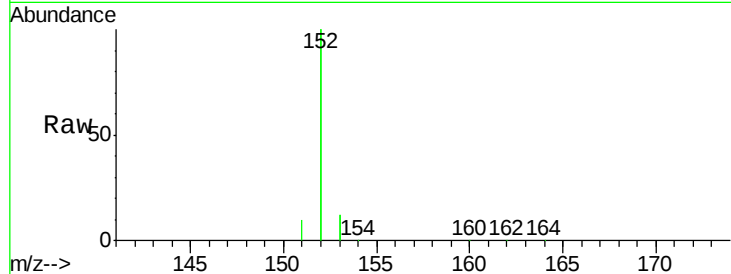

#16
Acenaphthene
Concen: 3.18 ng
RT: 14.82 min Scan# 980
Delta R.T. 0.00 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Lower	Upper
154	100		
153	460.6	350.8	526.2
152	229.4	171.1	256.7









#17
Fluorene
Concen: 3.25 ng
RT: 15.80 min Scan# 1044
Delta R.T. -0.01 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
166	100		
165	98.6	78.2	117.4
167	13.4	11.0	16.4




Manual Integrations
APPROVED


mohammad
3/7/2017 4:22:46 PM

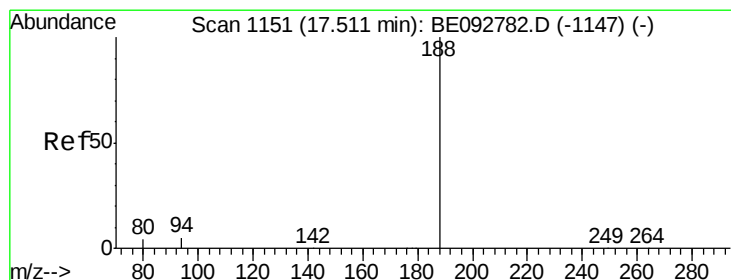

#18
Phenanthrene-d10
Concen: 5.00 ng
RT: 17.51 min Scan# 1151
Delta R.T. 0.00 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Lower	Upper
188	100		
94	3.0	3.2	4.8#
80	2.5	2.6	3.8#

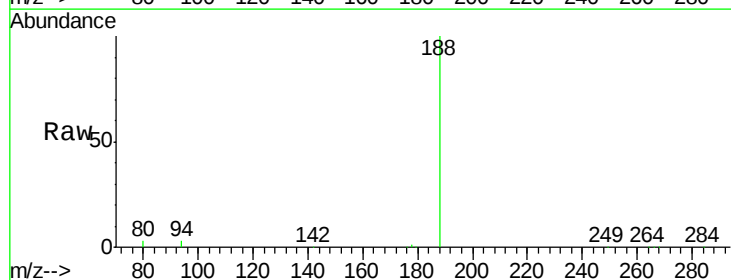







#19
Hexachlorobenzene
Concen: 3.63 ng
RT: 16.82 min Scan# 1121
Delta R.T. 0.00 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
284	100		
142	0.0	29.1	43.7#
249	31.7	27.9	41.9




Manual Integrations
APPROVED


mohammad
3/7/2017 4:22:46 PM

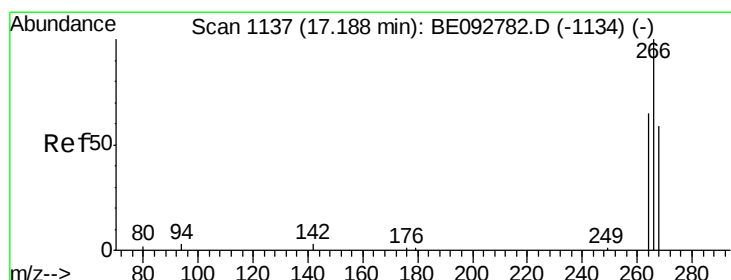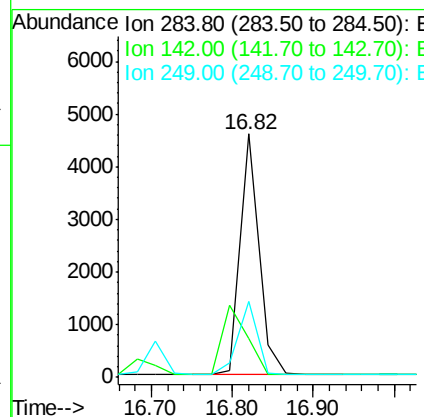

#20
Pentachlorophenol
Concen: 5.67 ng
RT: 17.17 min Scan# 1136
Delta R.T. -0.02 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Lower	Upper
266	100		
268	54.1	62.5	93.7#
264	74.6	57.2	85.8

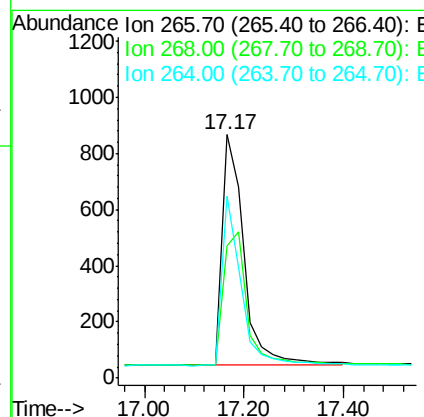



#21

Phenanthrene

Concen: 3.46 ng

RT: 17.53 min Scan# 1152

Delta R.T. -0.02 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Instrument :

BNA_E





ClientSampleId :

SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
178	100		
176	20.2	15.8	23.8
179	14.8	16.0	24.0

Manual Integrations
APPROVED

mohammad
3/7/2017 4:22:46 PM

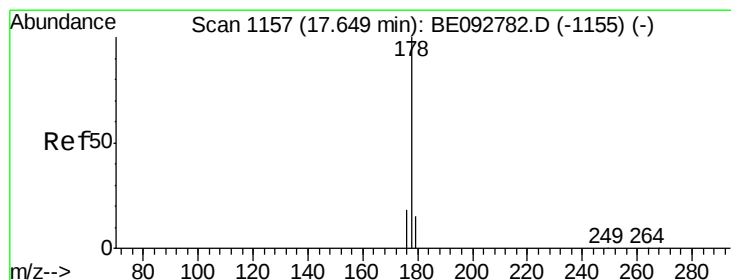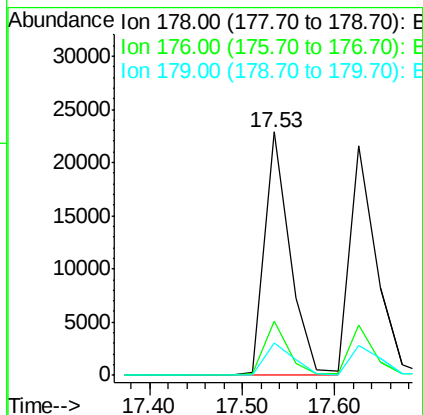

#22

Anthracene

Concen: 3.80 ng




RT: 17.63 min Scan# 1156


Delta R.T. -0.02 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Lower	Upper
178	100		
176	19.7	15.0	22.4
179	14.9	12.2	18.2

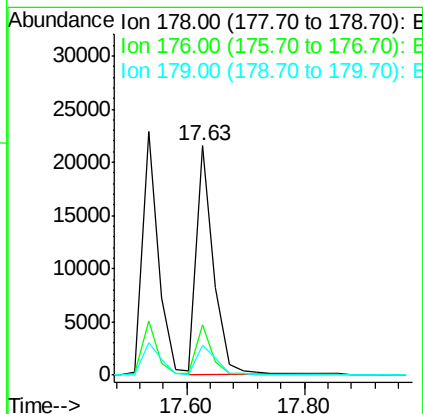







#23
 Fluoranthene
 Concen: 3.82 ng
 RT: 19.54 min Scan# 1262
 Delta R.T. -0.02 min
 Lab File: BE092785.D
 Acq: 6 Mar 2017 13:24

Instrument :
 BNA_E
 ClientSampleId :
 SSTDICC3.2

Tot Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	2.9	2.2	3.4
203	18.0	13.7	20.5




Manual Integrations
 APPROVED


mohammad
 3/7/2017 4:22:46 PM



#24
 Chrysene-d12
 Concen: 5.00 ng
 RT: 21.68 min Scan# 1372
 Delta R.T. 0.00 min
 Lab File: BE092785.D
 Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Resp Lower	Resp Upper
240	100		
120	2.6	2.6	4.0#
236	28.1	24.6	37.0









#25
Pvrene
Concen: 2.89 ng
RT: 19.90 min Scan# 1283
Delta R.T. -0.02 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Resp Lower	Upper
202	100		
200	5.3	4.2	6.4
203	17.2	13.9	20.9




Manual Integrations
APPROVED


mohammad
3/7/2017 4:22:46 PM

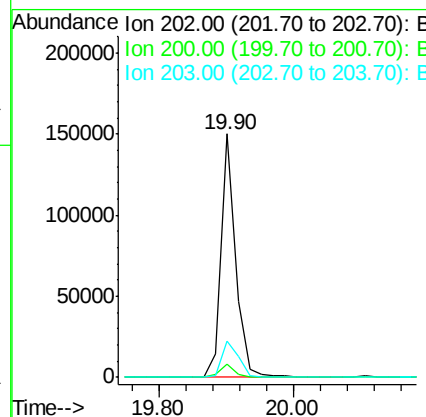

#26
Terphenyl-d14
Concen: 2.73 ng
RT: 20.11 min Scan# 1295
Delta R.T. -0.02 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Resp Lower	Upper
244	100		
212	10.3	6.7	10.1#
122	20.2	3.6	5.4#

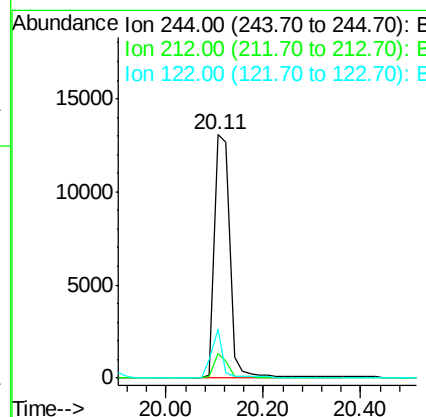







#27
Benzo(a)anthracene
Concen: 3.22 ng m
RT: 21.66 min Scan# 1371
Delta R.T. 0.00 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
228	100		
226	26.4	23.6	35.4
229	17.7	13.3	19.9




Manual Integrations
APPROVED


mohammad
3/7/2017 4:22:46 PM



#28
Chrysene
Concen: 2.47 ng m
RT: 21.70 min Scan# 1373
Delta R.T. -0.02 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Lower	Upper
228	100		
226	41.0	36.3	54.5
229	11.9	10.6	16.0





#29

Bis(2-ethylhexyl)phthalate

Concen: 1.75 ng

RT: 21.59 min Scan# 1368

Delta R.T. 0.00 min

Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Instrument :

BNA_E


ClientSampleId :

SSTDICC3.2




Tot Ion:	149	Resp:	19263
Ion Ratio	Lower	Upper	
149	100		
167	28.9	16.0	24.0#
279	3.4	16.0	24.0#

Manual Integrations
APPROVED

mohammad
3/7/2017 4:22:46 PM



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

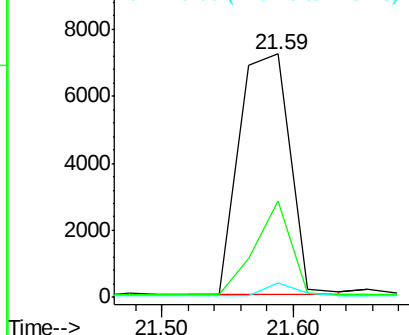

#30

Indeno(1,2,3-cd)pyrene

Concen: 2.50 ng

RT: 26.45 min Scan# 1707




Delta R.T. -0.03 min


Lab File: BE092785.D

Acq: 6 Mar 2017 13:24

Tgt Ion:	276	Resp:	264484
Ion Ratio	Lower	Upper	
276	100		
138	28.1	20.3	30.5
277	24.8	19.7	29.5

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

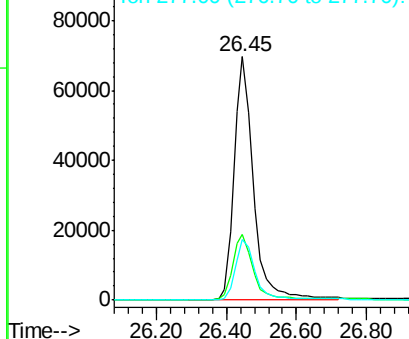

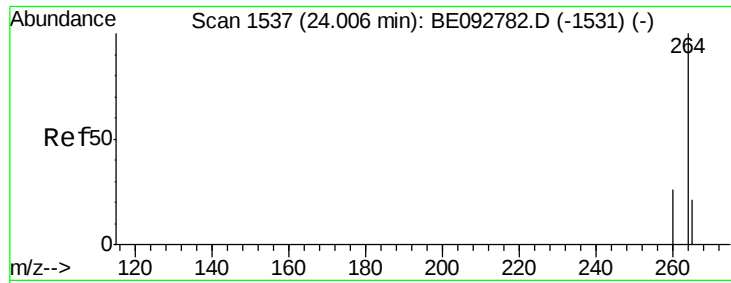





#31
Pervlene-d12
Concen: 5.00 ng
RT: 24.01 min Scan# 1537
Delta R.T. 0.00 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.6	20.1	30.1
265	21.8	17.9	26.9




Manual Integrations
APPROVED


mohammad
3/7/2017 4:22:46 PM



#32
Benzo(b)fluoranthene
Concen: 3.14 ng
RT: 23.28 min Scan# 1474
Delta R.T. -0.01 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Lower	Upper
252	100		
253	19.8	18.7	28.1
125	11.8	10.5	15.7



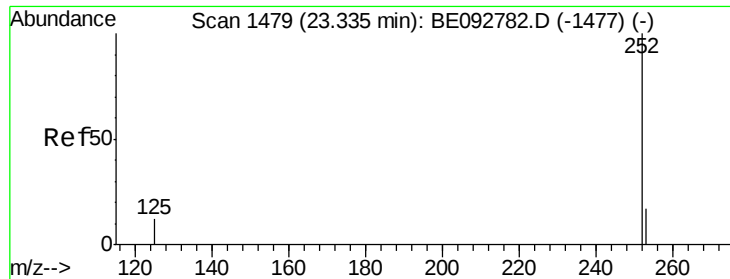





#33
Benzo(k)fluoranthene
Concen: 2.65 ng
RT: 23.34 min Scan# 1479
Delta R.T. 0.00 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.9	20.3	30.5
125	9.8	9.6	14.4




Manual Integrations
APPROVED


mohammad
3/7/2017 4:22:46 PM

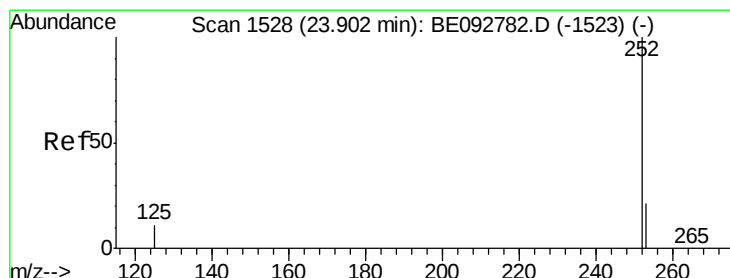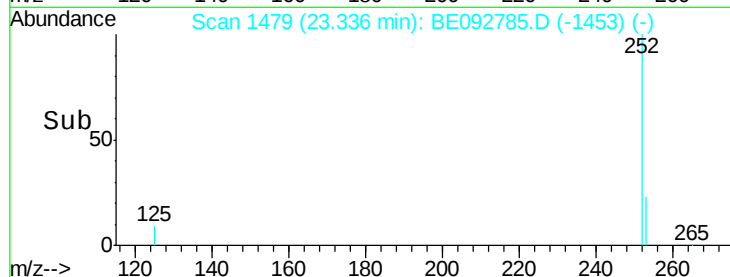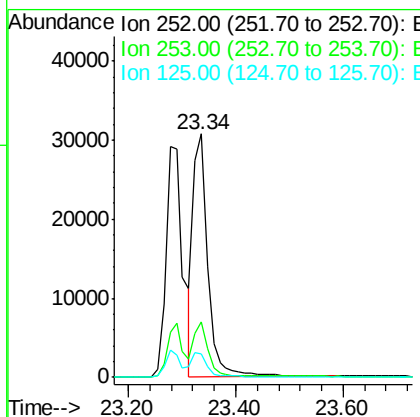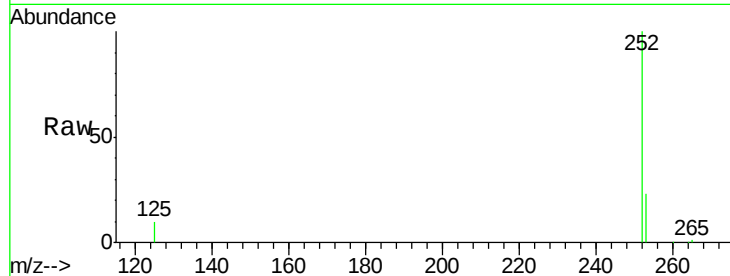

#34
Benzo(a)pyrene
Concen: 3.13 ng
RT: 23.89 min Scan# 1527
Delta R.T. -0.01 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.0	19.0	28.6
125	12.4	11.8	17.8

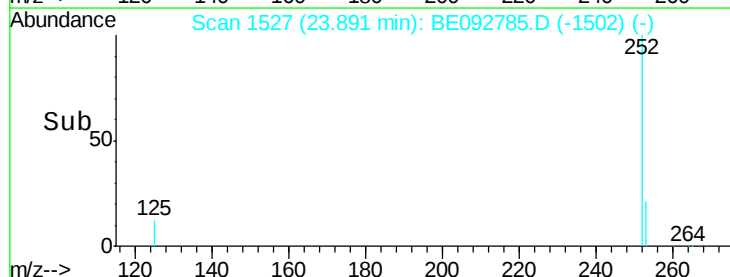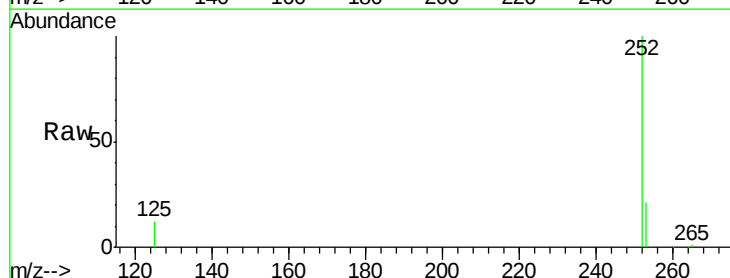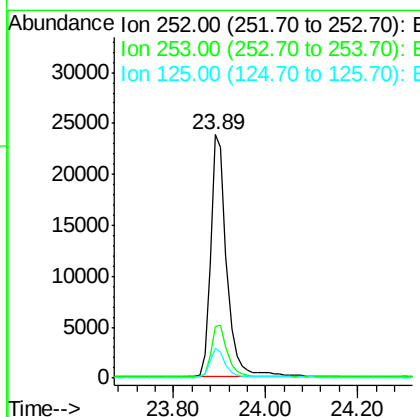







#35
Dibenzo(a,h)anthracene
Concen: 2.86 ng
RT: 26.46 min Scan# 1708
Delta R.T. -0.03 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Instrument :
BNA_E
ClientSampleId :
SSTDICC3.2

Tot Ion	Ratio	Lower	Upper
278	100		
139	18.4	13.8	20.8
279	23.0	21.4	32.2

Manual Integrations
APPROVED

mohammad
3/7/2017 4:22:46 PM



#36
Benzo(g,h,i)perylene
Concen: 2.81 ng
RT: 27.20 min Scan# 1751
Delta R.T. -0.03 min
Lab File: BE092785.D
Acq: 6 Mar 2017 13:24

Tgt Ion	Ratio	Lower	Upper
276	100		
277	23.0	19.8	29.8
138	25.1	19.8	29.6

