


Data Path : Z:\HPCHEM1\BNA E\DATA\BE030617\
 Data File : BE092779.D
 Acq On : 6 Mar 2017 9:37
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 06 15:46:01 2017

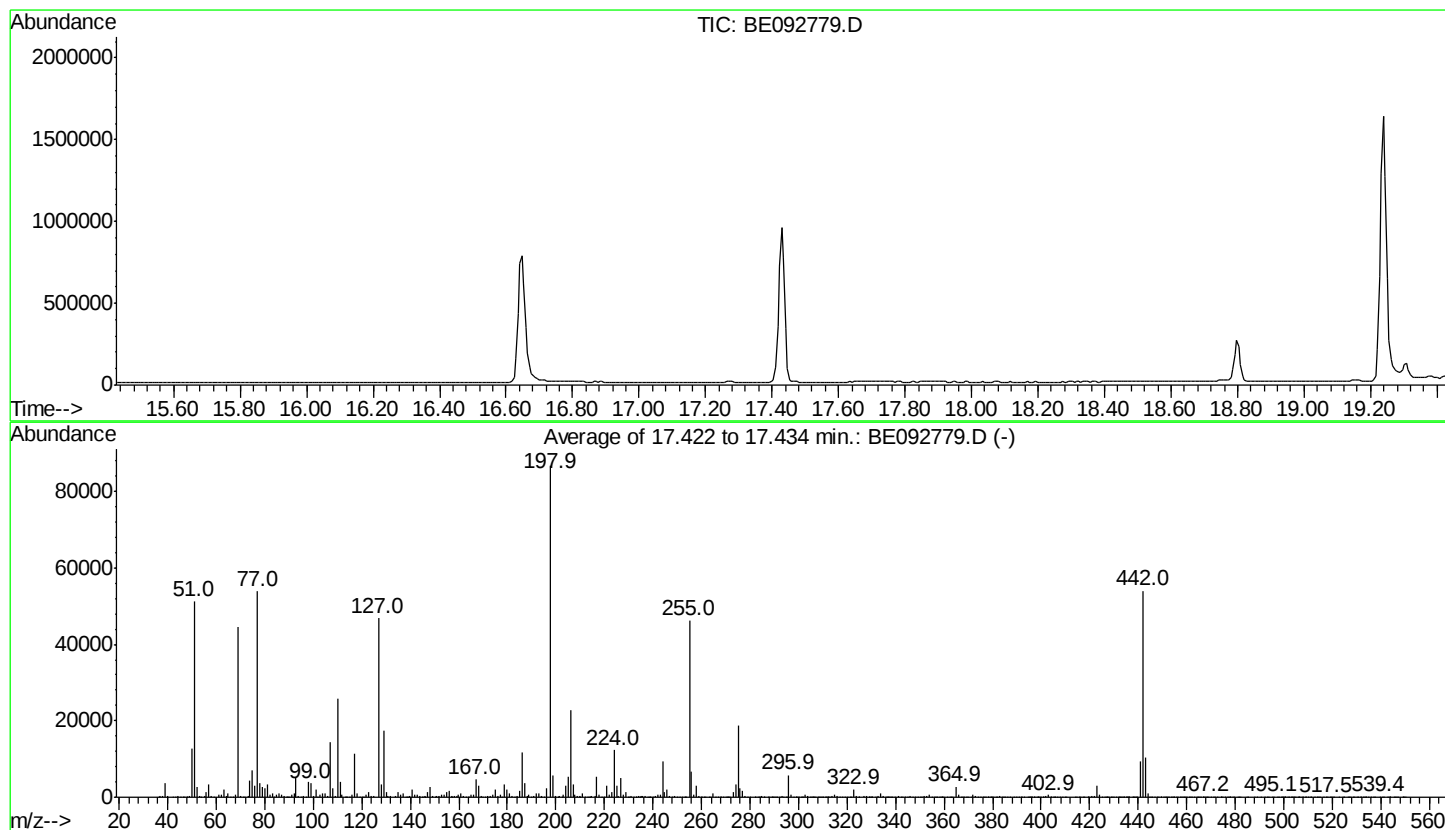

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.0	51151	PASS
68	69	0.00	2	1.2	528	PASS
69	198	0.00	100	51.5	44703	PASS
70	69	0.00	2	0.6	266	PASS
127	198	10	80	54.0	46875	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	86750	PASS
199	198	5	9	6.8	5859	PASS
275	198	10	60	21.5	18629	PASS
365	198	1	100	3.2	2745	PASS
441	442	0.01	24	17.1	9256	PASS
442	198	50	100	62.3	54084	PASS
443	442	15	24	19.5	10544	PASS