
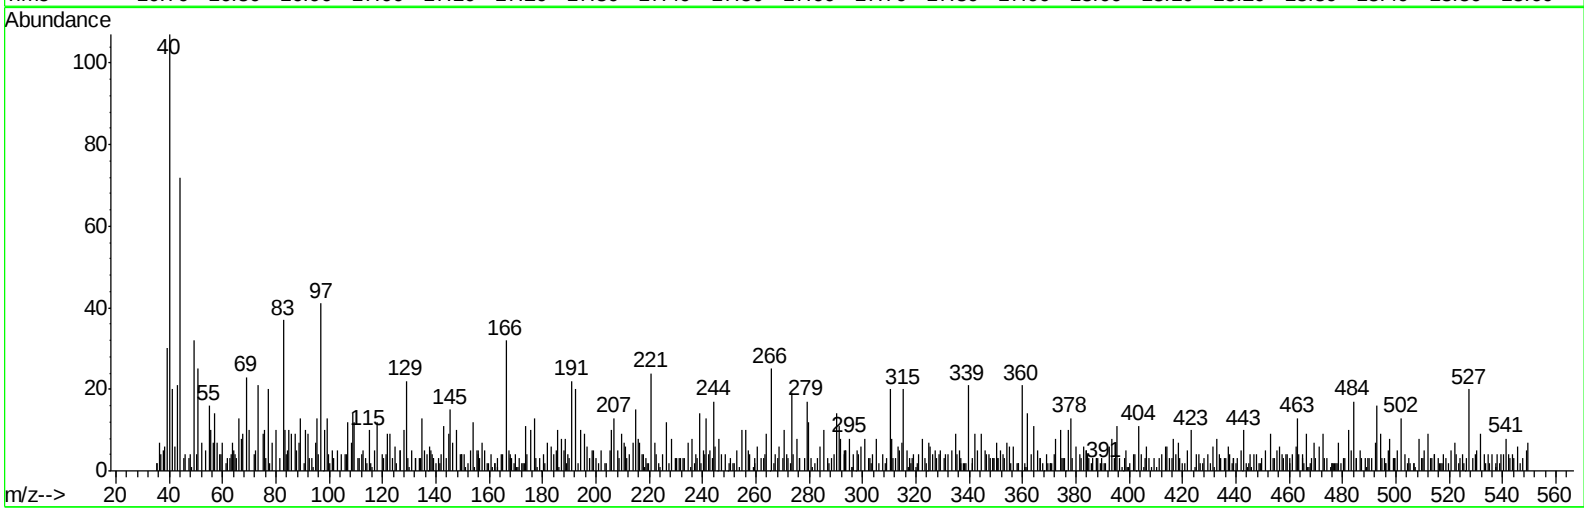


Data Path : Z:\HPCHEM1\BNA E\Data\BE030618\
Data File : BE095699.D
Acq On : 6 Mar 2018 16:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 03:41:12 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 06 11:52:59 2018
Response via : Initial Calibration

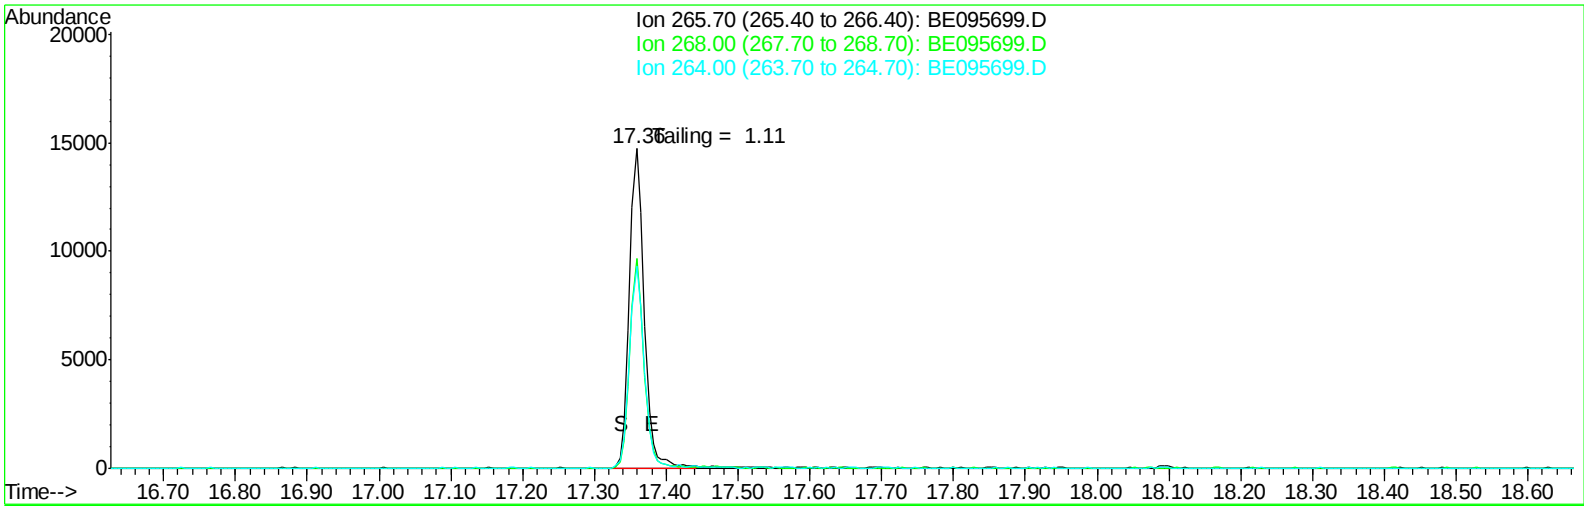




TIC: BE095699.D

(69) Pentachlorophenol (C)
10.901min (-0.320) 418.10ng
response 16

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	12.00#
264.00	61.90	36.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE030618\
Data File : BE095699.D
Acq On : 6 Mar 2018 16:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 03:41:12 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 06 11:52:59 2018
Response via : Initial Calibration

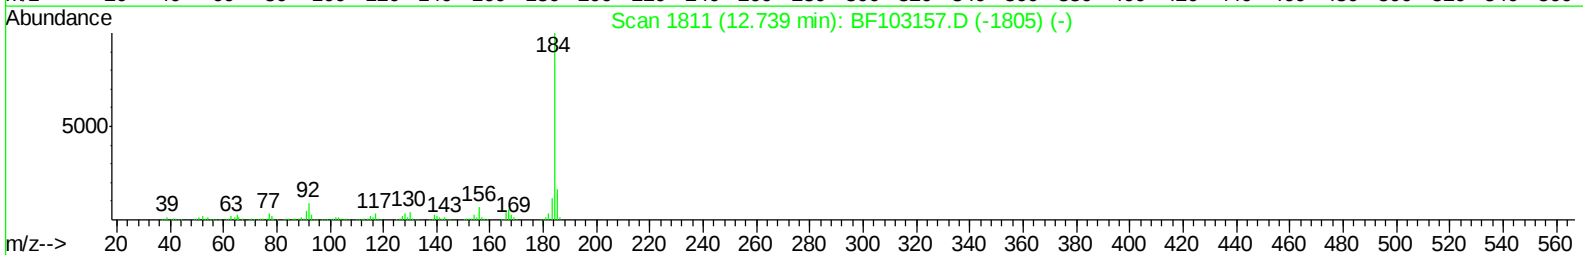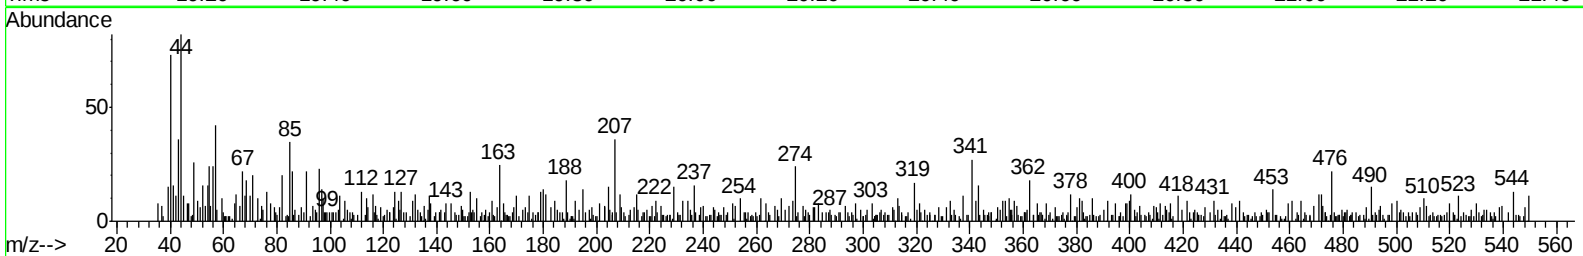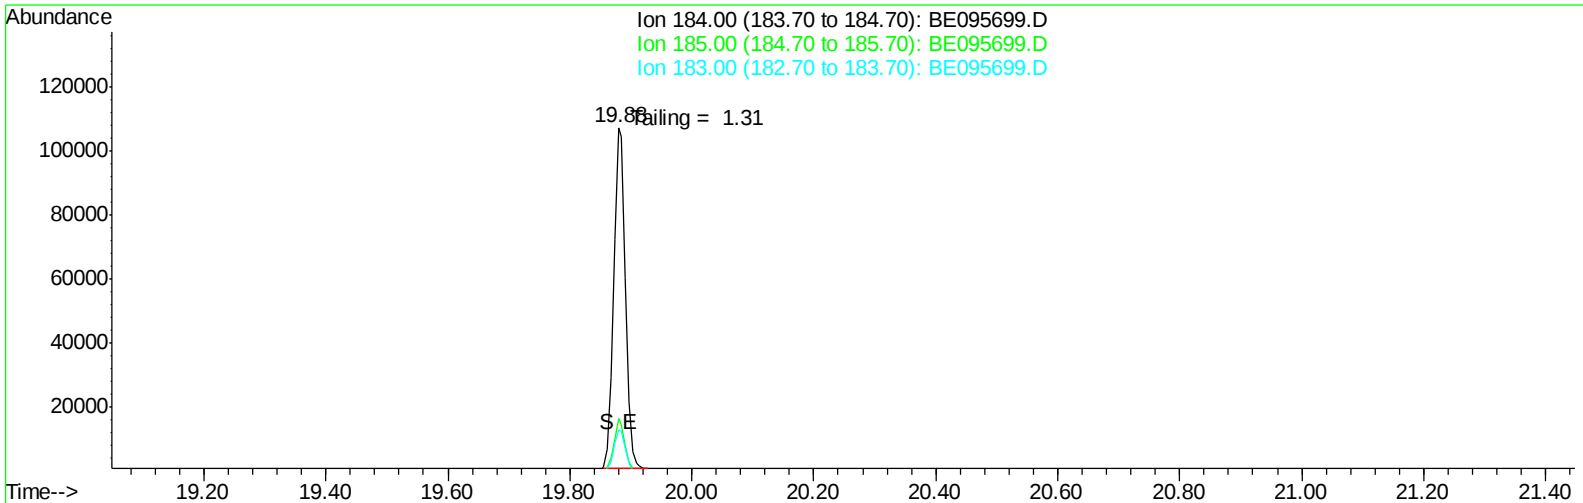

TIC: BE095699.D

(76) Benzidine

12.400min (-0.351) 5.94ng

response 4

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	55.56#
183.00	11.60	66.67#
0.00	0.00	0.00