


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE030618\
Data File : BE095699.D
Acq On : 6 Mar 2018 16:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE022318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 23 12:12:42 2018

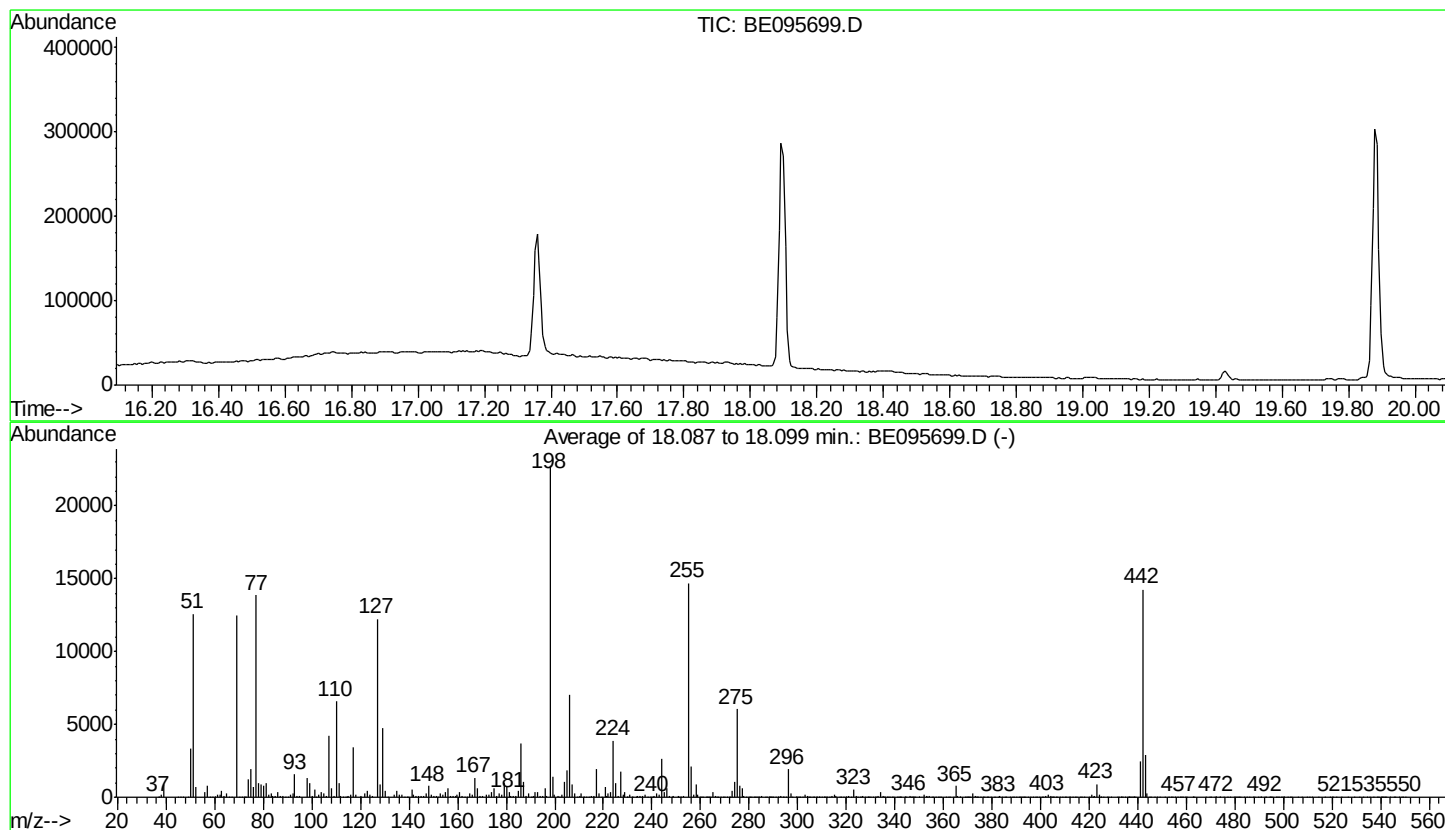

AutoFind: Scans 2638, 2639, 2640; Background Corrected with Scan 2630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.4	12608	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	54.7	12449	PASS
70	69	0.00	2	0.2	30	PASS
127	198	10	80	53.9	12258	PASS
197	198	0.00	2	0.3	72	PASS
198	198	100	100	100.0	22760	PASS
199	198	5	9	6.3	1435	PASS
275	198	10	60	26.5	6024	PASS
365	198	1	100	3.3	760	PASS
441	442	0.01	24	17.0	2421	PASS
442	198	50	100	62.6	14242	PASS
443	442	15	24	20.3	2886	PASS