
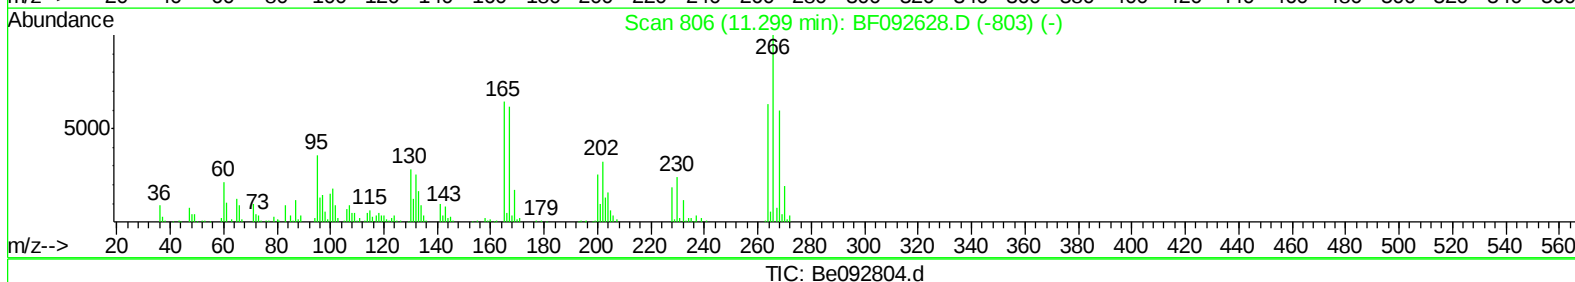
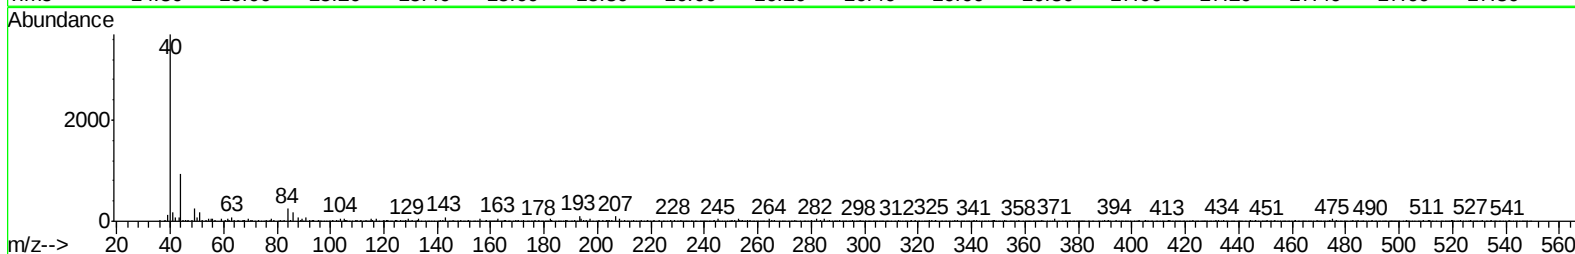


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE030717\
Data File : Be092804.d
Acq On : 7 Mar 2017 9:03
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 16:05:51 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

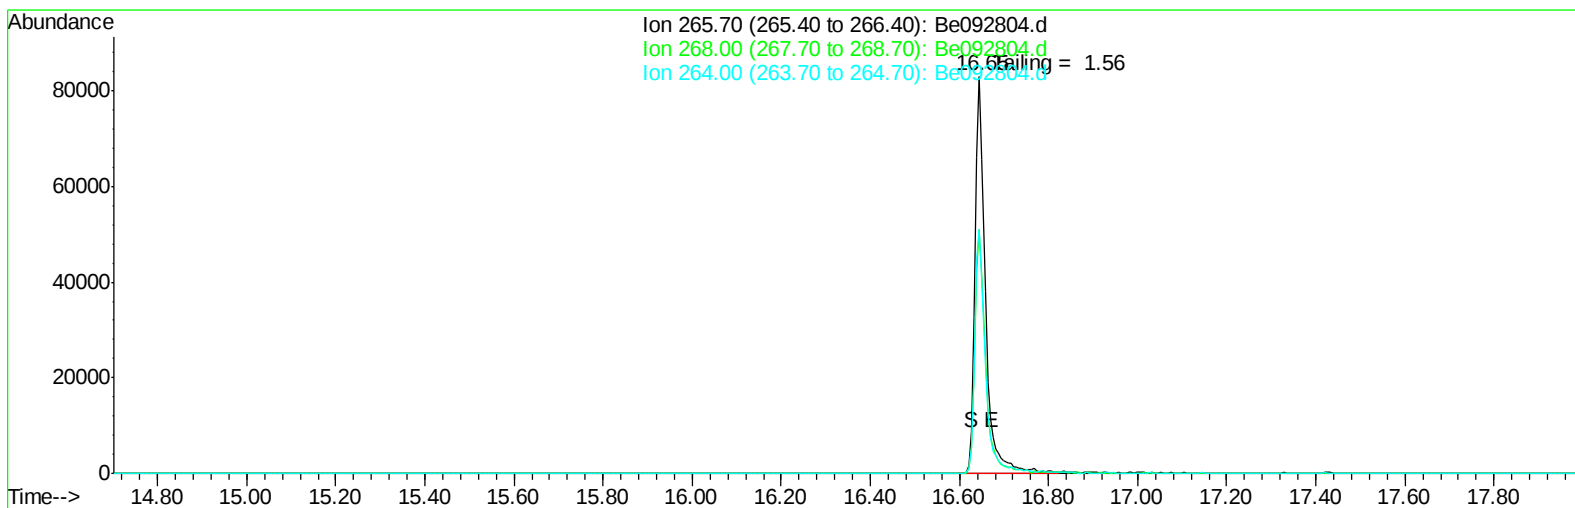

TIC: Be092804.d

(69) Pentachlorophenol (C)




11.017min (-0.168) 34.16ng

response 6

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	33.33#
264.00	62.90	228.57#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE030717\
 Data File : Be092804.d
 Acq On : 7 Mar 2017 9:03
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 16:05:51 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 17:31:55 2017
 Response via : Initial Calibration

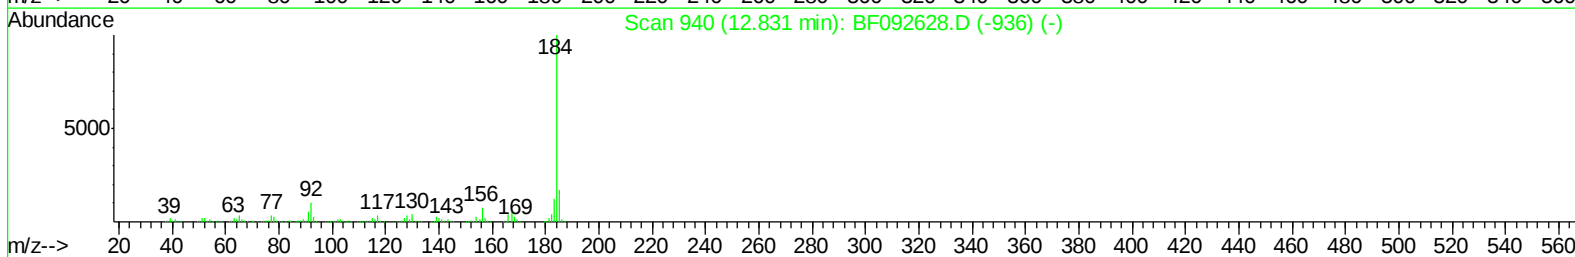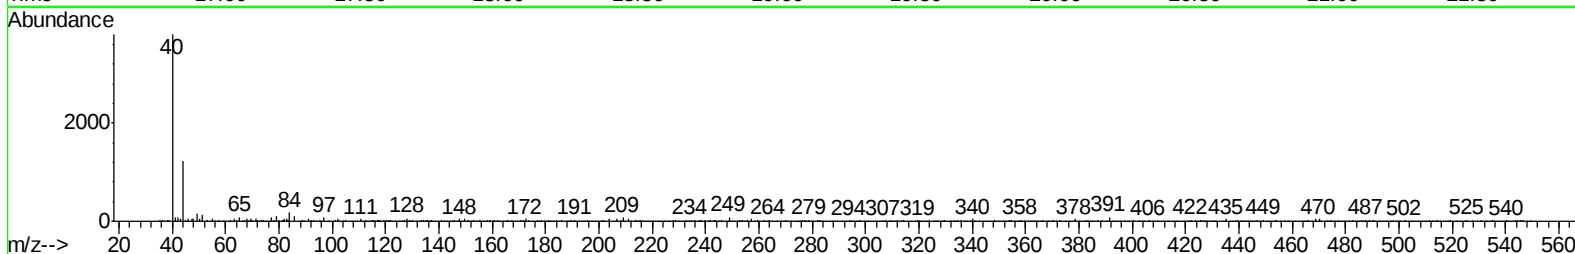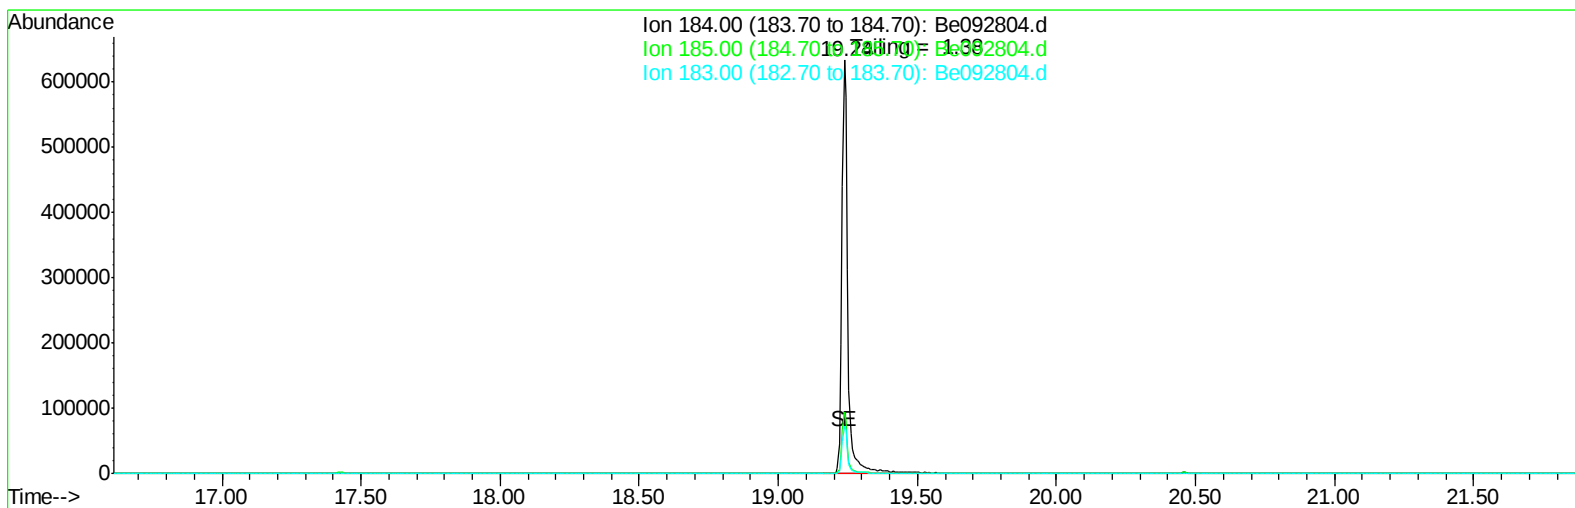

TIC: Be092804.d

(76) Benzidine

12.327min (-0.390) 17.60ng

response 15

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	20.00
183.00	11.50	12.00
0.00	0.00	0.00