


Data Path : Z:\HPCHEM1\BNA E\DATA\BE030717\
Data File : BE092804.D
Acq On : 7 Mar 2017 9:03
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030617.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 06 15:46:01 2017

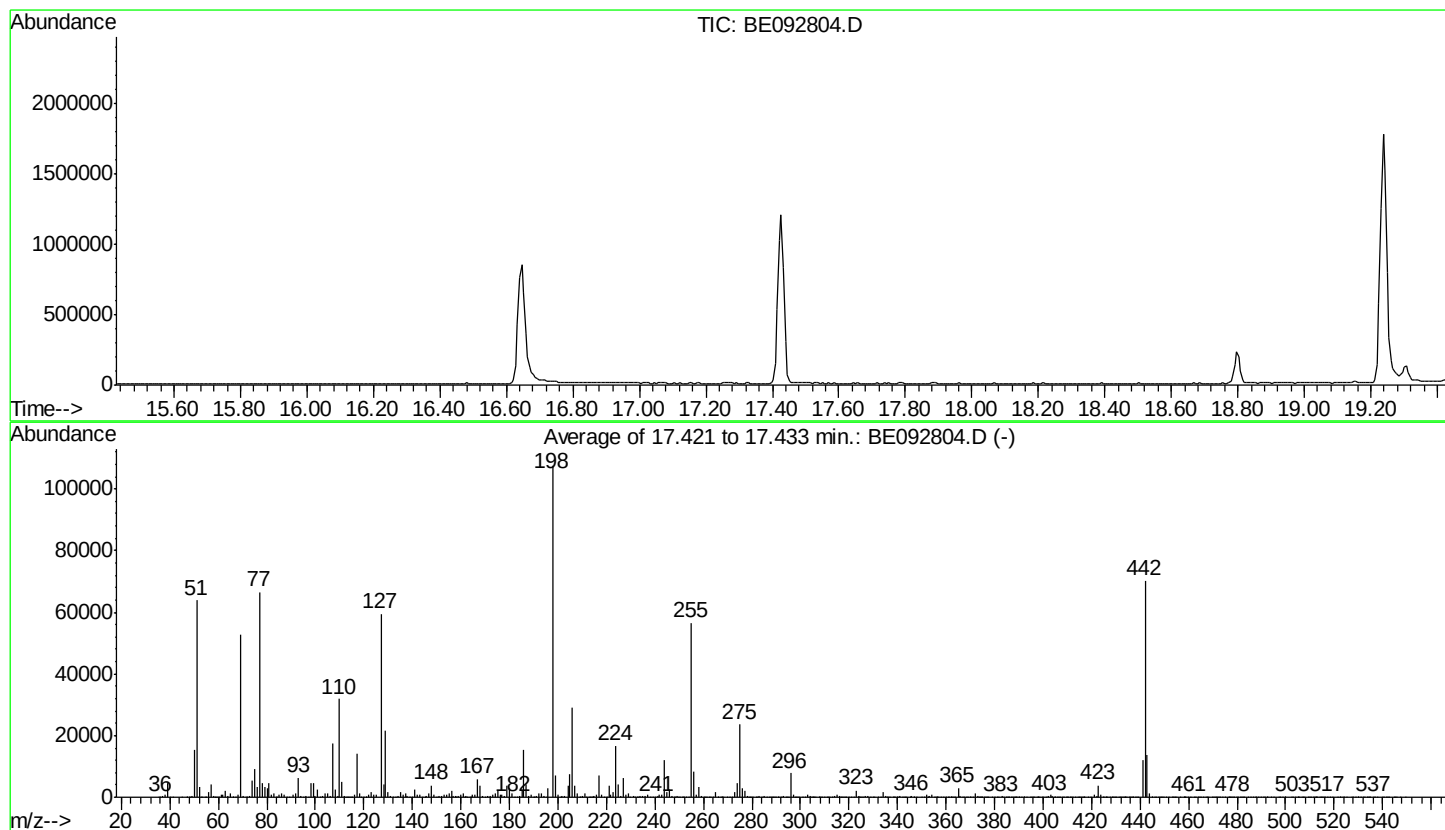

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.3	63765	PASS
68	69	0.00	2	1.6	843	PASS
69	198	0.00	100	49.2	52899	PASS
70	69	0.00	2	0.6	341	PASS
127	198	10	80	55.3	59452	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	107576	PASS
199	198	5	9	6.7	7229	PASS
275	198	10	60	21.9	23578	PASS
365	198	1	100	2.8	2990	PASS
441	442	0.01	24	17.3	12164	PASS
442	198	50	100	65.3	70229	PASS
443	442	15	24	19.8	13894	PASS