


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE030718\
 Data File : BE095717.D
 Acq On : 7 Mar 2018 11:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE022318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 23 12:12:42 2018

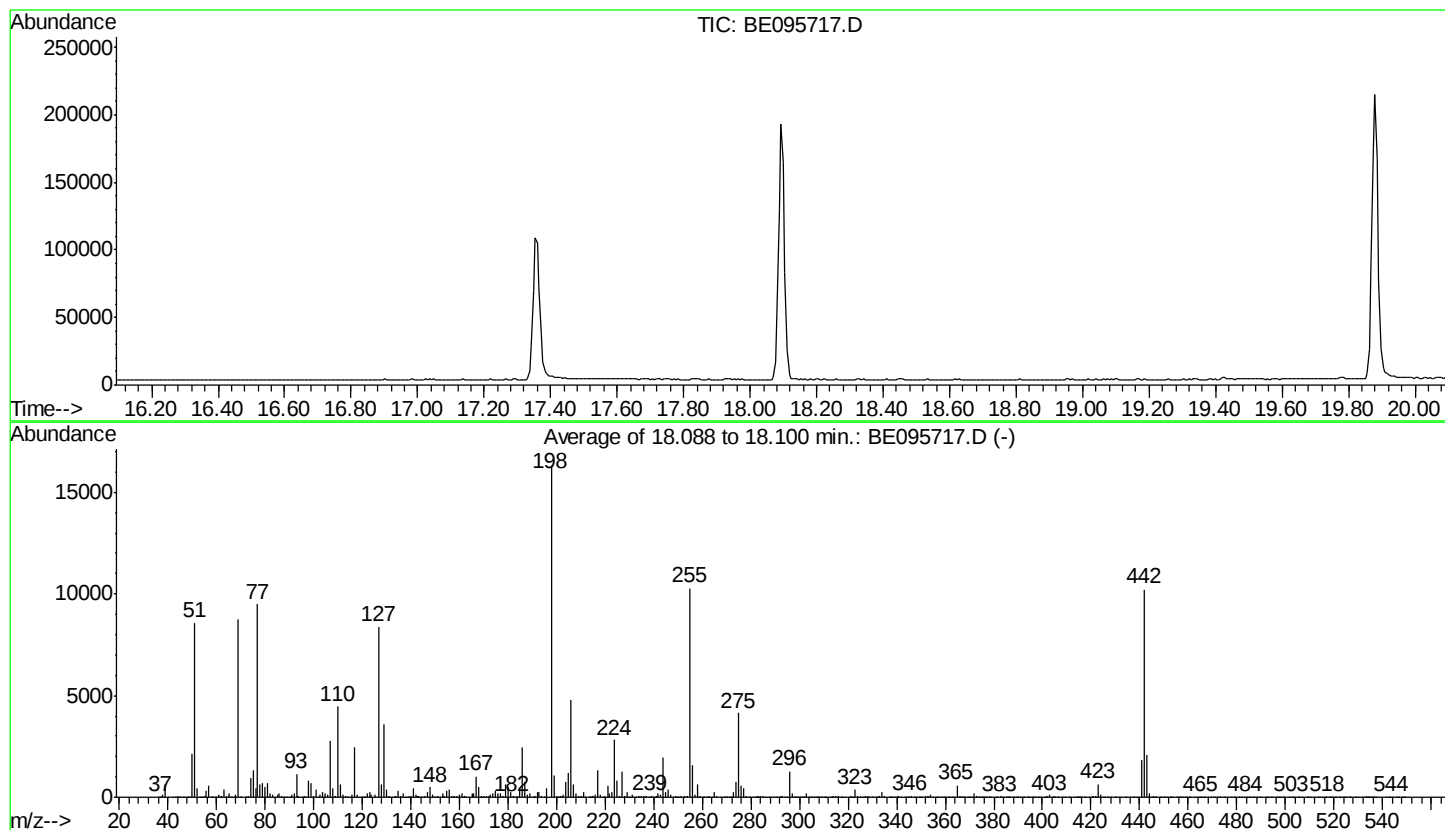

AutoFind: Scans 2638, 2639, 2640; Background Corrected with Scan 2629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.7	8592	PASS
68	69	0.00	2	1.2	101	PASS
69	198	0.00	100	53.8	8776	PASS
70	69	0.00	2	0.3	22	PASS
127	198	10	80	51.4	8377	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16311	PASS
199	198	5	9	6.6	1077	PASS
275	198	10	60	25.4	4150	PASS
365	198	1	100	3.7	598	PASS
441	442	0.01	24	17.7	1806	PASS
442	198	50	100	62.5	10201	PASS
443	442	15	24	20.2	2064	PASS