


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE030719\
 Data File : BE098810.D
 Acq On : 7 Mar 2019 8:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 06 15:33:24 2019

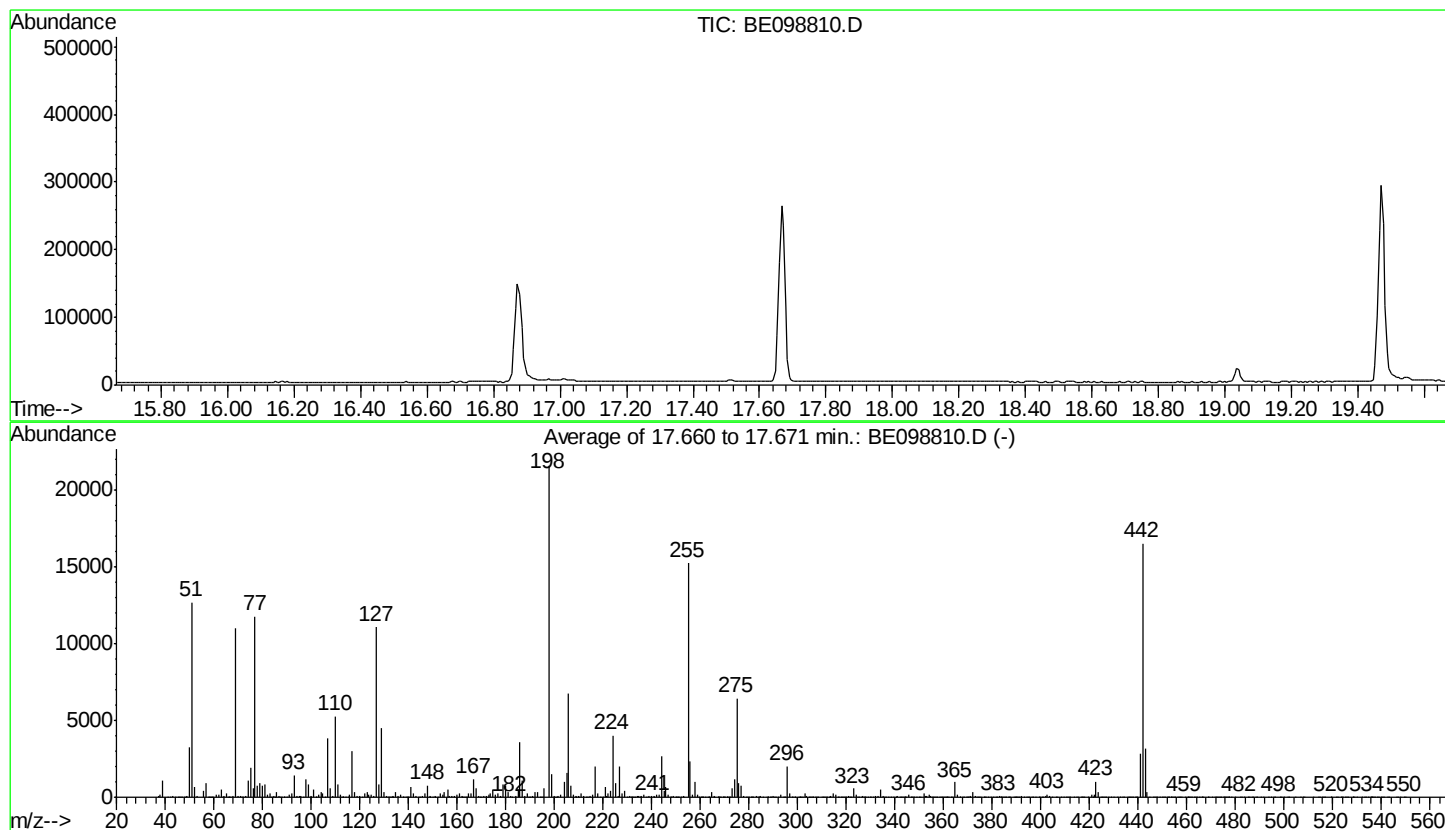

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2557

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.7	12655	PASS
68	69	0.00	2	0.9	94	PASS
69	198	0.00	100	50.9	10976	PASS
70	69	0.00	2	0.5	51	PASS
127	198	10	80	51.5	11091	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	21555	PASS
199	198	5	9	7.1	1539	PASS
275	198	10	60	29.9	6447	PASS
365	198	1	100	4.5	960	PASS
441	198	0.01	100	13.0	2800	PASS
442	198	50	100	76.5	16493	PASS
443	442	15	24	19.4	3202	PASS