
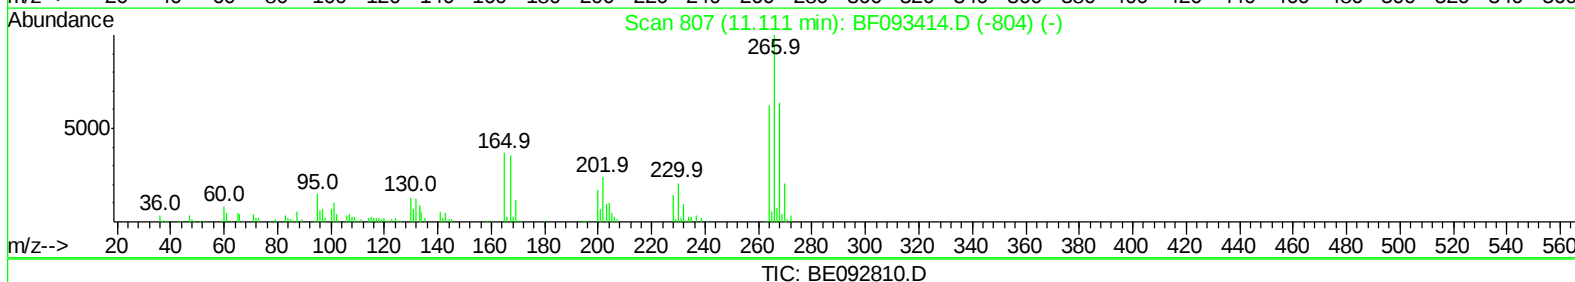
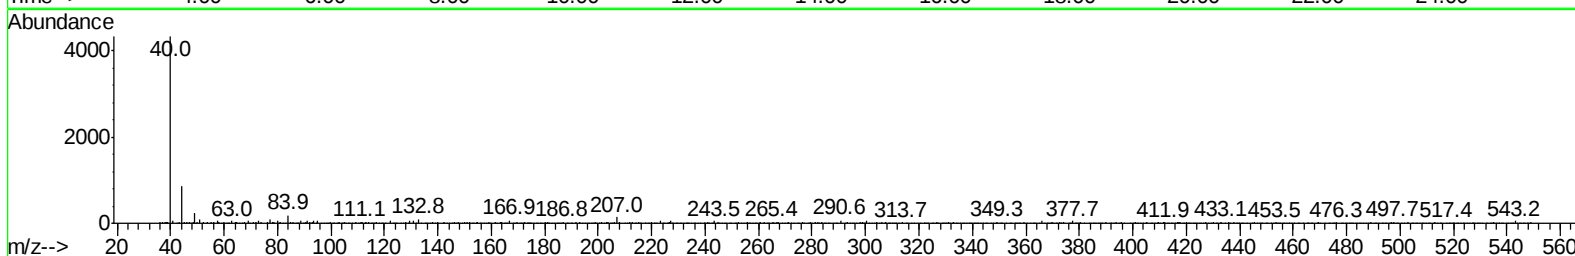


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031017\
Data File : BE092810.D
Acq On : 10 Mar 2017 16:34
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 22:07:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

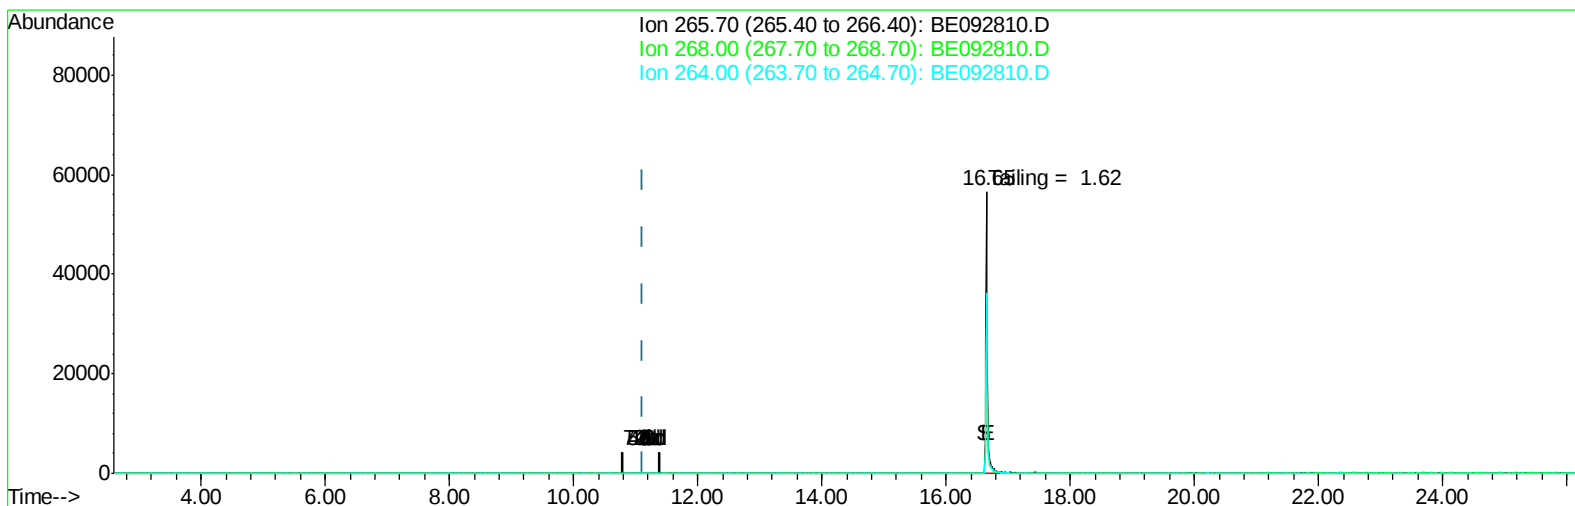

TIC: BE092810.D

(69) Pentachlorophenol (C)




11.130min (+0.020) 627.46ng

response 35

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	16.67#
264.00	62.90	18.75#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031017\
Data File : BE092810.D
Acq On : 10 Mar 2017 16:34
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 22:07:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 07 15:55:22 2017
Response via : Initial Calibration

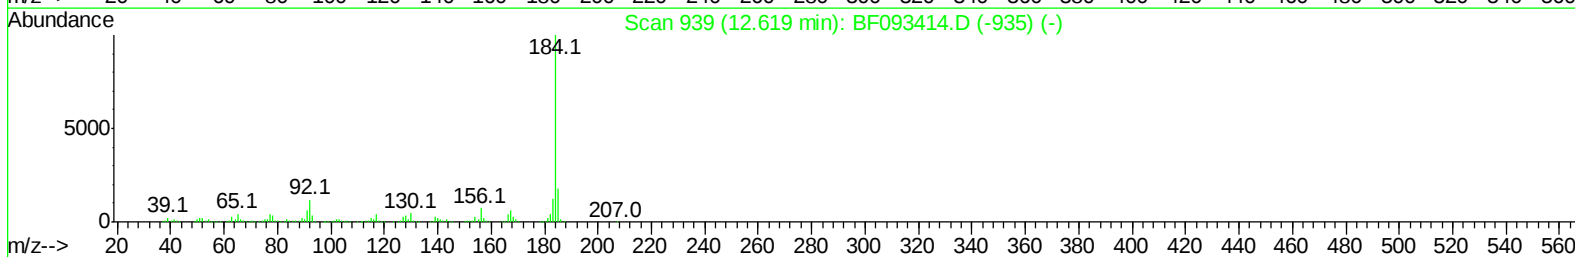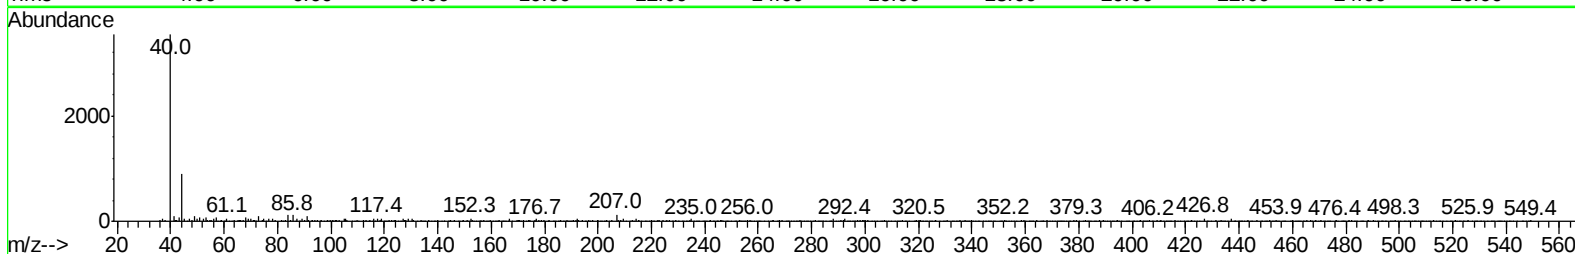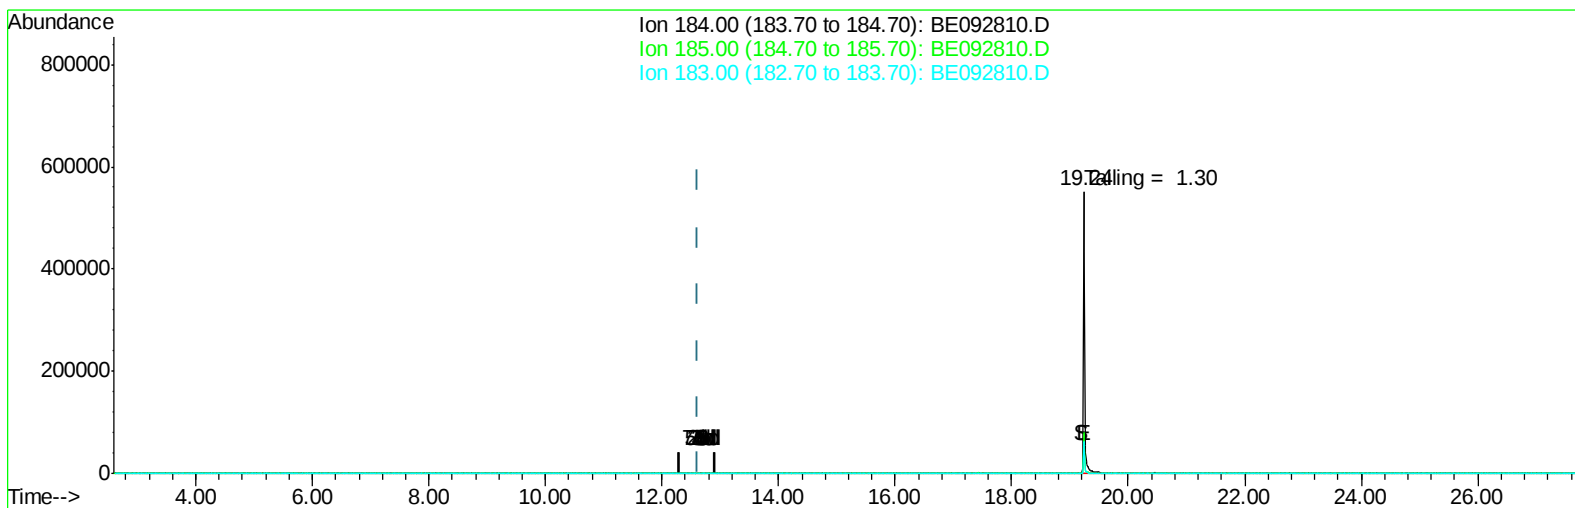

TIC: BE092810.D

(76) Benzidine

12.681min (+0.062) 3.86ng

response 8

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	62.50#
183.00	11.50	75.00#
0.00	0.00	0.00