


Data Path : Z:\HPCHEM1\BNA_E\Data\BE031017\
 Data File : BE092810.D
 Acq On : 10 Mar 2017 16:34
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 06 15:46:01 2017

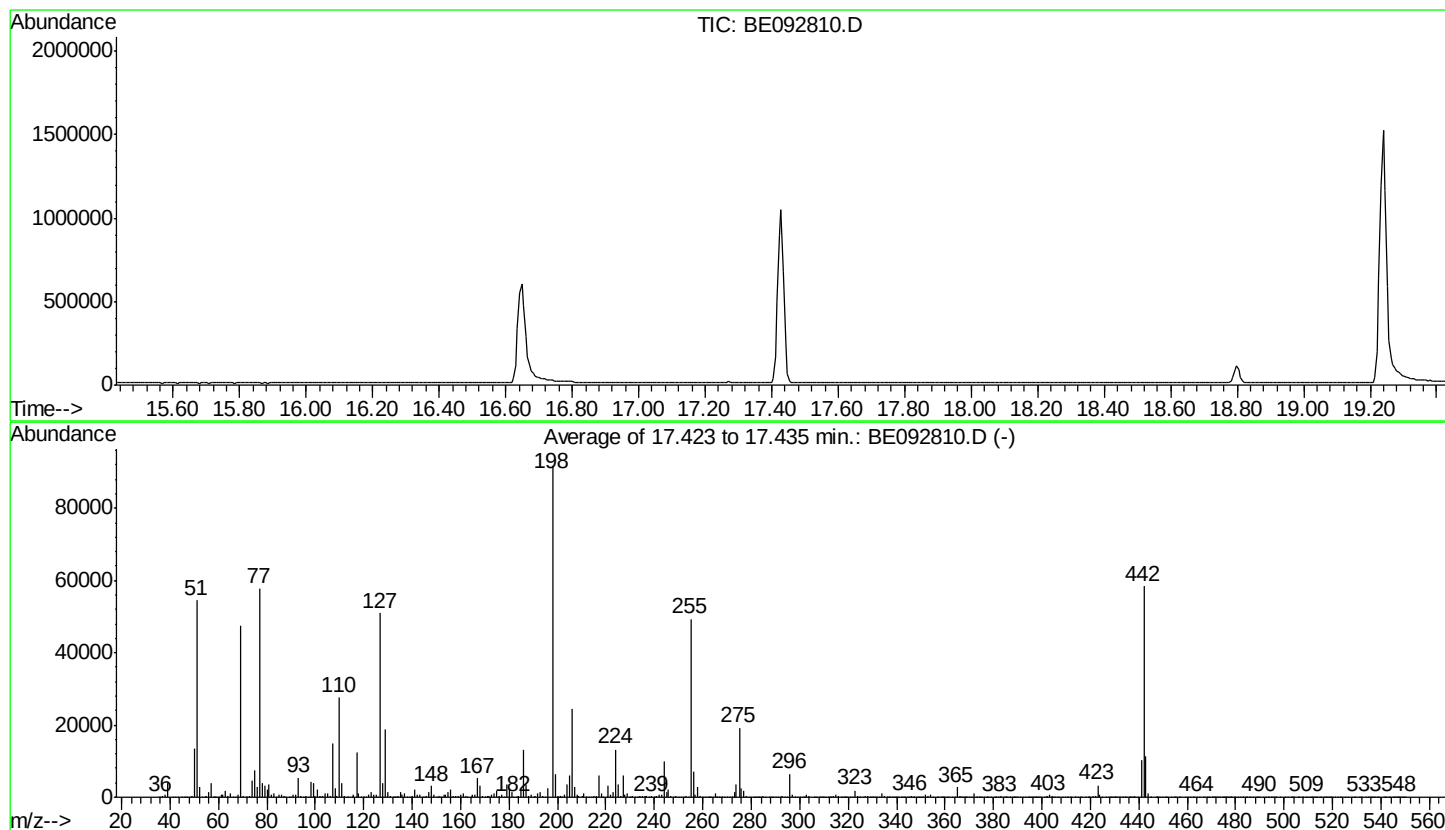

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.3	54492	PASS
68	69	0.00	2	1.4	672	PASS
69	198	0.00	100	51.6	47344	PASS
70	69	0.00	2	0.6	263	PASS
127	198	10	80	55.5	51000	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	91823	PASS
199	198	5	9	6.8	6260	PASS
275	198	10	60	20.9	19162	PASS
365	198	1	100	3.0	2717	PASS
441	442	0.01	24	17.8	10373	PASS
442	198	50	100	63.6	58415	PASS
443	442	15	24	19.2	11222	PASS