

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031218\
 Data File : BE095727.D
 Acq On : 12 Mar 2018 13:14
 Operator : SJ/JU
 Sample : J1867-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 CPS093071

Quant Time: Mar 12 14:42:42 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE022318.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 23 12:12:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1678	0.40	ng	0.00
7) Naphthalene-d8	11.27	136	6588	0.40	ng	0.00
13) Acenaphthene-d10	15.00	164	4608	0.40	ng	0.00
19) Phenanthrene-d10	17.71	188	8631	0.40	ng	0.00
27) Chrysene-d12	21.80	240	8722	0.40	ng	0.00
34) Perylene-d12	24.43	264	8194	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.92	112	776	0.18	ng	0.00
5) Phenol-d6	7.56	99	727	0.12	ng	0.00
8) Nitrobenzene-d5	9.61	82	2697	0.40	ng	0.00
11) 2-Methylnaphthalene-d10	12.80	152	4079	0.37	ng	0.00
14) 2,4,6-Tribromophenol	16.47	330	736	0.45	ng	0.00
15) 2-Fluorobiphenyl	13.64	172	6909	0.34	ng	0.00
25) Fluoranthene-d10	19.69	212	42669	0.38	ng	0.00
29) Terphenyl-d14	20.25	244	6853	0.39	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Naphthalene	11.31	128	44727	0.589	ng	# 96
12) 2-Methylnaphthalene	12.87	142	31273	2.387	ng	# 97
17) Acenaphthene	15.06	154	2163	0.133	ng	# 56
18) Fluorene	16.03	166	4532	0.225	ng	# 81
22) Pentachlorophenol	17.37	266	360391	175.119	ng	# 71
23) Phenanthrene	17.75	178	1481	0.055	ng	# 96
32) Bis(2-ethylhexyl)phthalate	21.66	149	7786	0.155	ng	# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE031218\
Data File : BE095727.D
Acq On : 12 Mar 2018 13:14
Operator : SJ/JU
Sample : J1867-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
CPS093071

Quant Time: Mar 12 14:42:42 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE022318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 12:12:42 2018
Response via : Initial Calibration

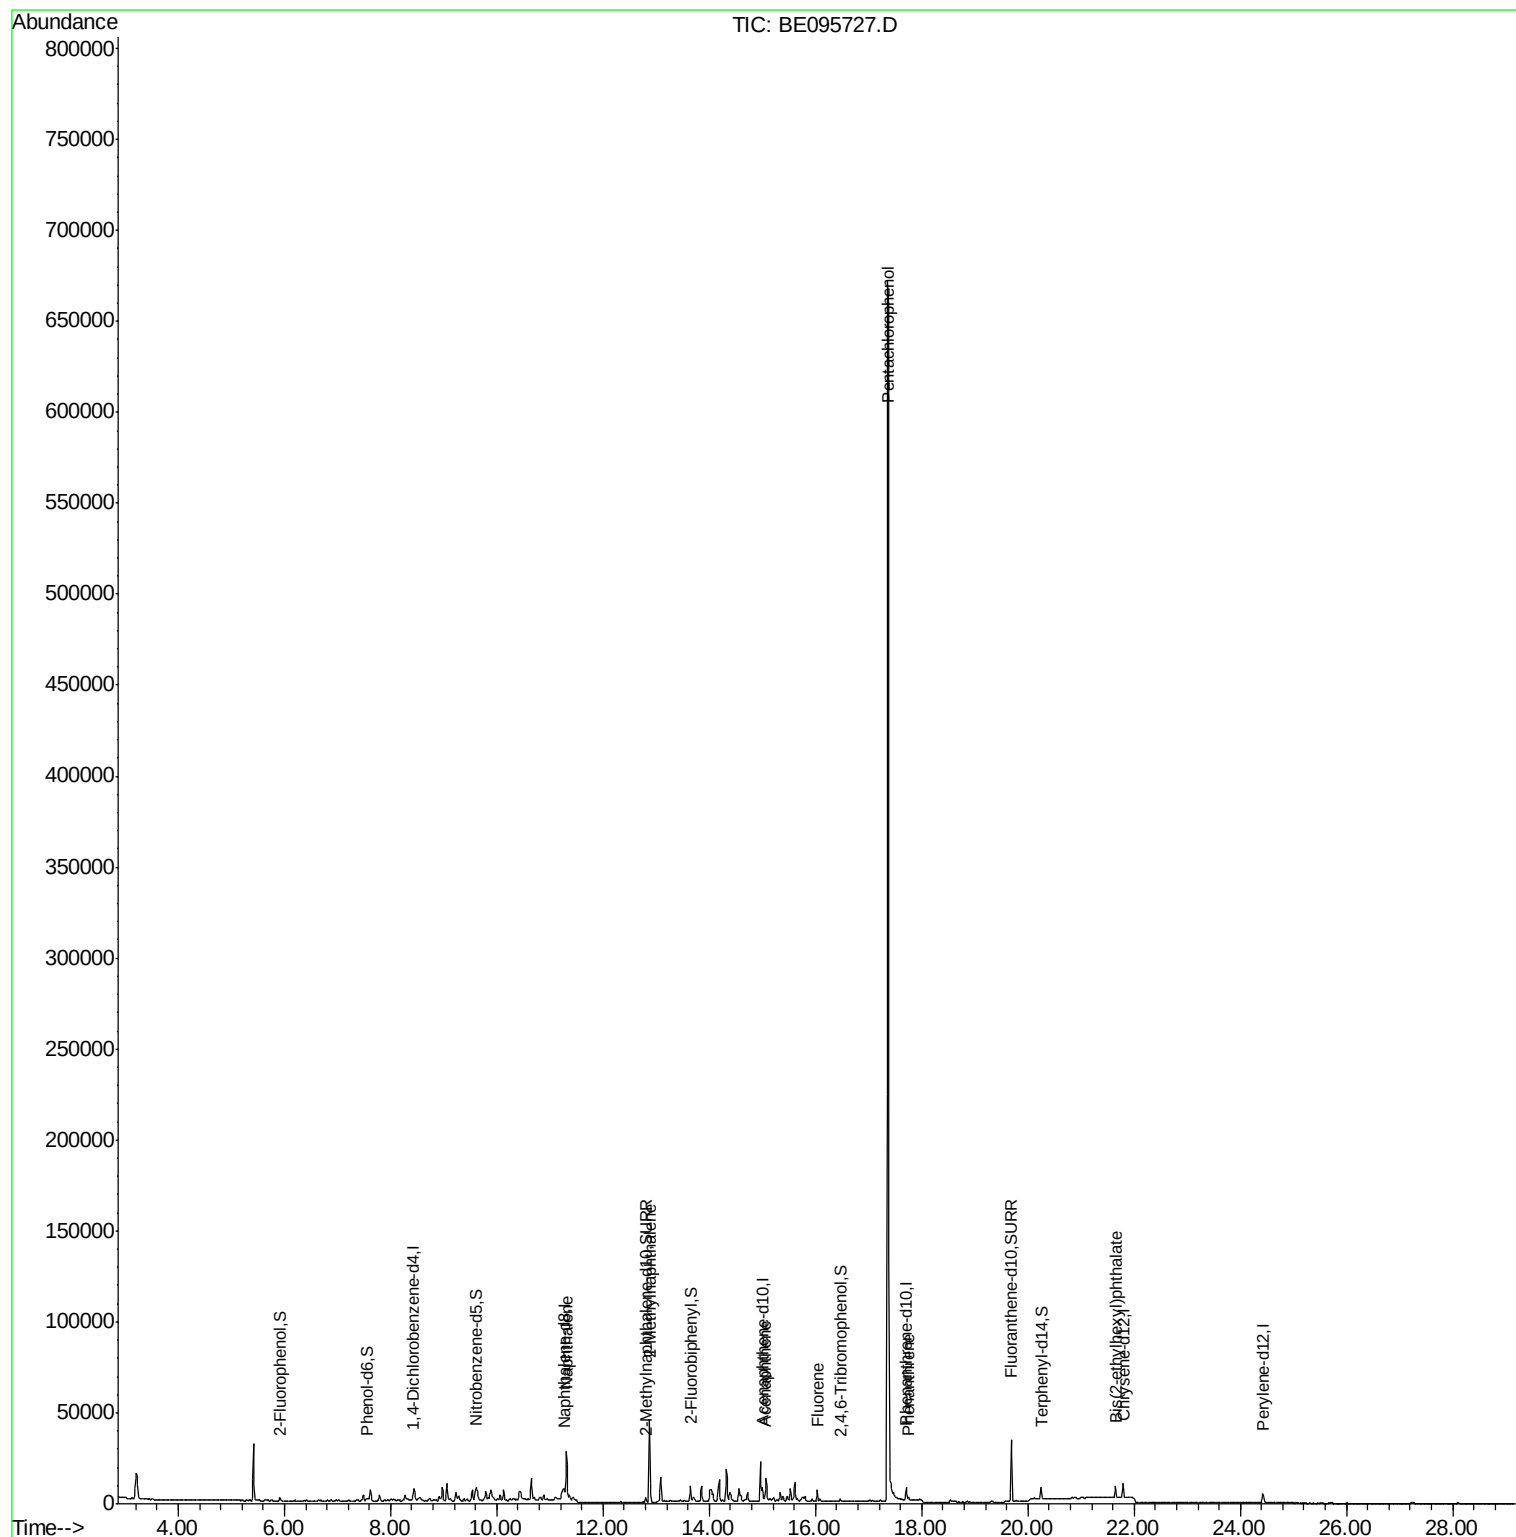



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 8.43 min Scan# 569

Delta R.T. -0.01 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14

Instrument :

BNA_E

ClientSampleId :

CPS093071


Tot Ion:152 Resp: 1678

Ion Ratio Lower Upper

152 100

150 143.3 117.2 175.8




115 72.1 57.0 85.6

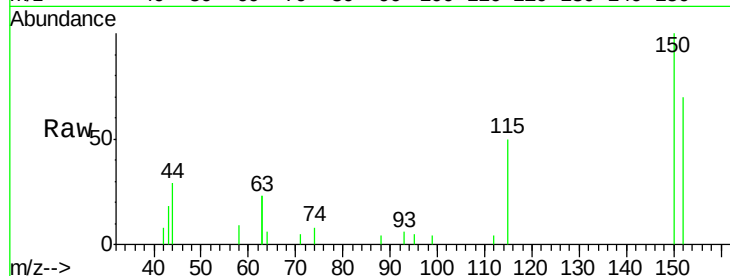

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

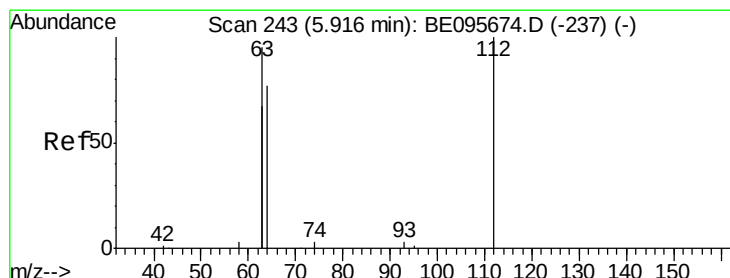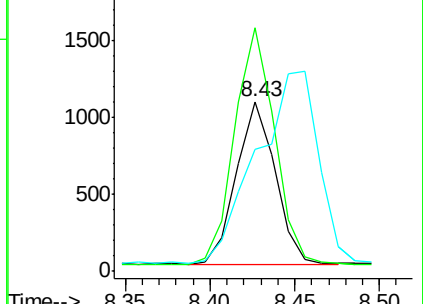

#4

2-Fluorophenol

Concen: 0.175 ng

RT: 5.92 min Scan# 313

Delta R.T. 0.01 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14


Tgt Ion:112 Resp: 776

Ion Ratio Lower Upper

112 100

64 74.4 60.1 90.1



63 156.2 116.8 175.2

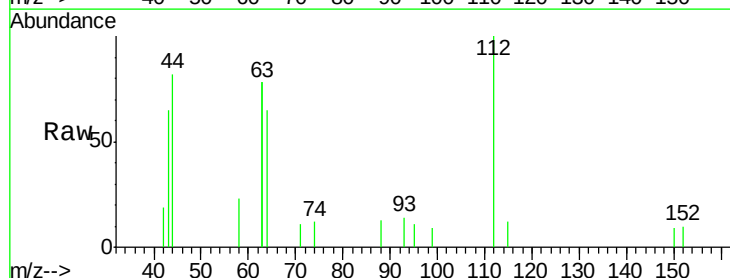


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

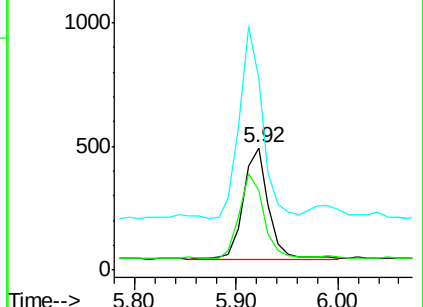

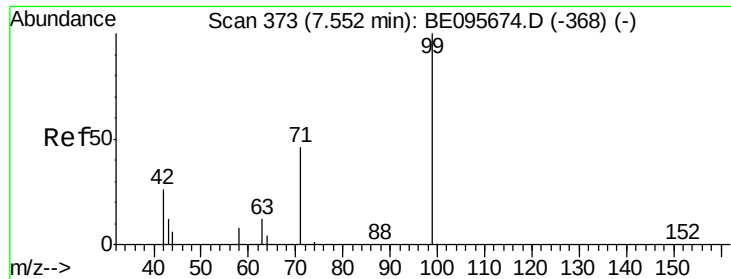

#5

Phenol-d6

Concen: 0.119 ng

RT: 7.56 min Scan# 480

Delta R.T. 0.00 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14

Instrument :

BNA_E

ClientSampleId :

CPS093071


Tot Ion: 99 Resp: 727

Ion Ratio Lower Upper

99 100

42 38.7 20.2 30.2#




71 50.2 28.4 42.6#

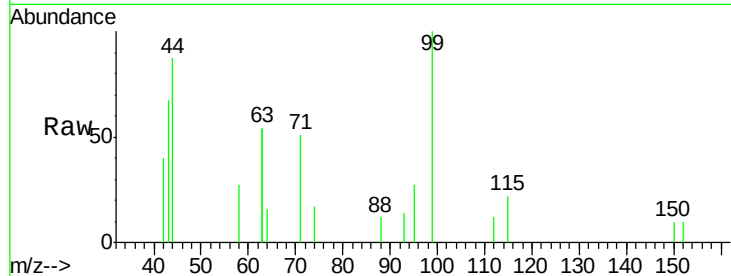

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

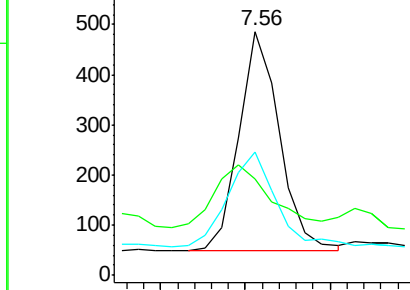

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 11.27 min Scan# 785

Delta R.T. -0.01 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14

Tgt Ion:136 Resp: 6588


Ion Ratio Lower Upper

136 100

137 11.5 9.5 14.3

54 30.8 29.1 43.7

68 6.5 6.2 9.2






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

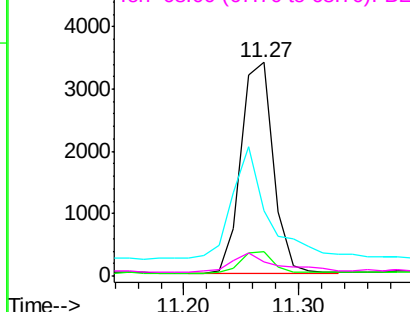



#8

Nitrobenzene-d5

Concen: 0.397 ng

RT: 9.61 min Scan# 657

Delta R.T. -0.01 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14

Instrument :

BNA_E

ClientSampled :

CPS093071


Tot Ion: 82 Resp: 2697

Ion Ratio Lower Upper

82 100

128 138.3 150.0 225.0#




54 208.2 154.2 231.4

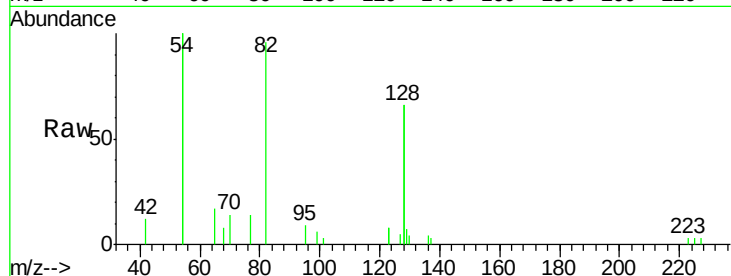

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

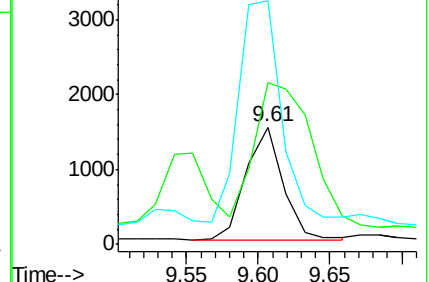

#9

Naphthalene

Concen: 0.589 ng

RT: 11.31 min Scan# 788

Delta R.T. -0.00 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14


Tgt Ion: 128 Resp: 44727

Ion Ratio Lower Upper

128 100

129 5.0 2.6 3.8#



127 4.1 2.8 4.2




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E



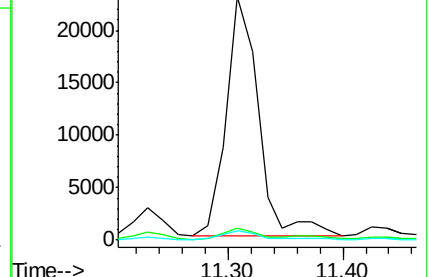



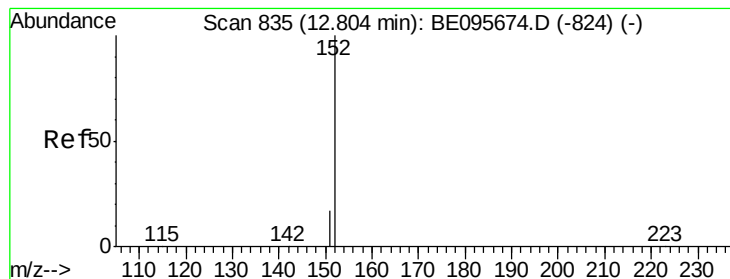

#11
 2-Methylnaphthalene-d10
 Concen: 0.370 ng
 RT: 12.80 min Scan# 1073
 Delta R.T. -0.00 min
 Lab File: BE095727.D
 Acq: 12 Mar 2018 13:14




Instrument :
 BNA_E
 ClientSampleId :
 CPS093071


Tot Ion:152 Resp: 4079
 Ion Ratio Lower Upper
 152 100
 151 19.8 15.4 23.0

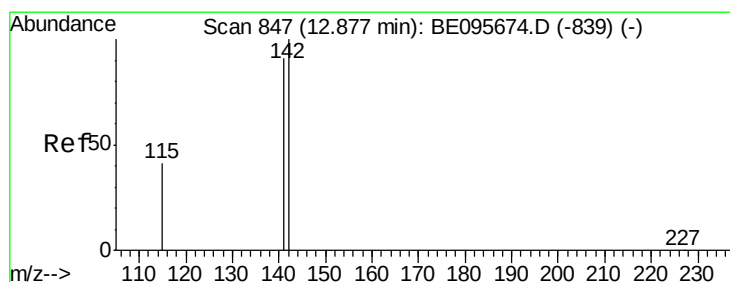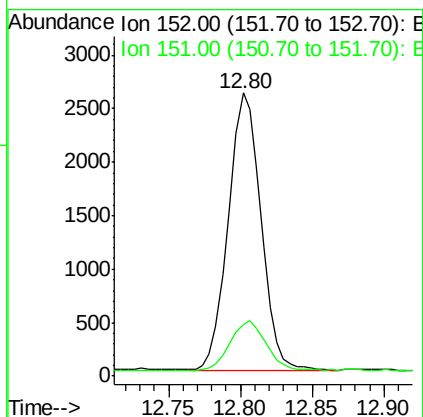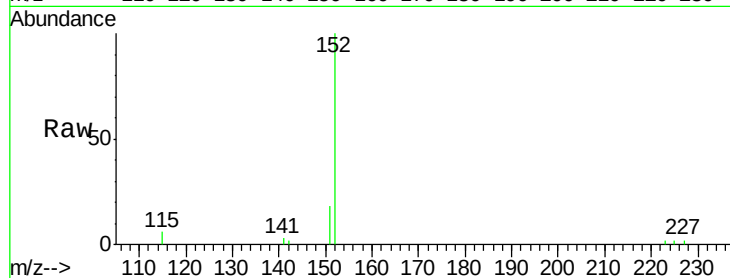

#12
 2-Methylnaphthalene
 Concen: 2.387 ng
 RT: 12.87 min Scan# 1088
 Delta R.T. -0.00 min
 Lab File: BE095727.D
 Acq: 12 Mar 2018 13:14

Tgt Ion:142 Resp: 31273
 Ion Ratio Lower Upper
 142 100
 141 90.6 70.4 105.6
 115 42.7 31.7 47.5

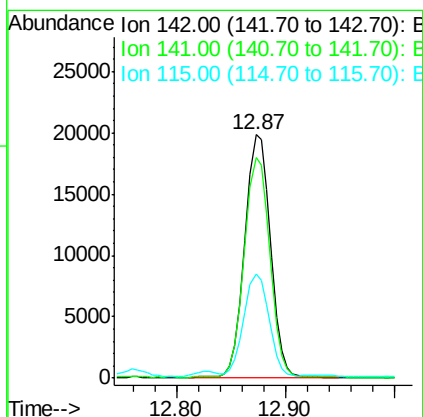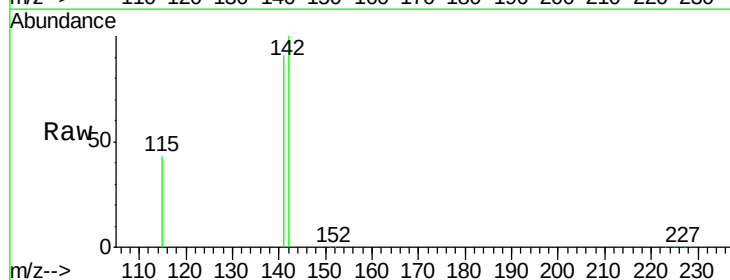



#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 15.00 min Scan# 1286

Delta R.T. 0.00 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14

Instrument :

BNA_E

ClientSampleId :

CPS093071


Tot Ion:164 Resp: 4608

Ion Ratio Lower Upper

164 100

162 107.1 83.1 124.7




160 54.4 37.1 55.7

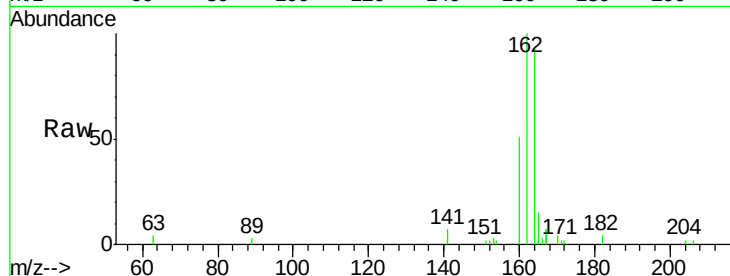

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

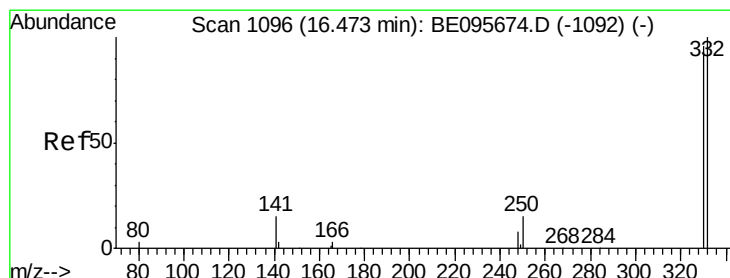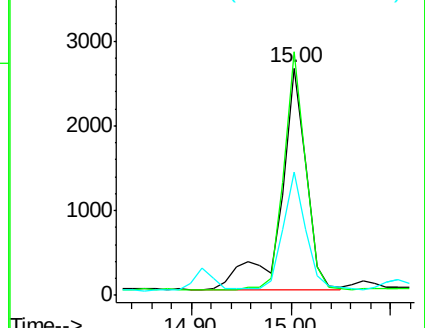

#14

2,4,6-Tribromophenol

Concen: 0.449 ng

RT: 16.47 min Scan# 1409

Delta R.T. -0.00 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14


Tgt Ion:330 Resp: 736

Ion Ratio Lower Upper

330 100

332 94.7 152.7 229.1#



141 60.2 33.7 50.5#

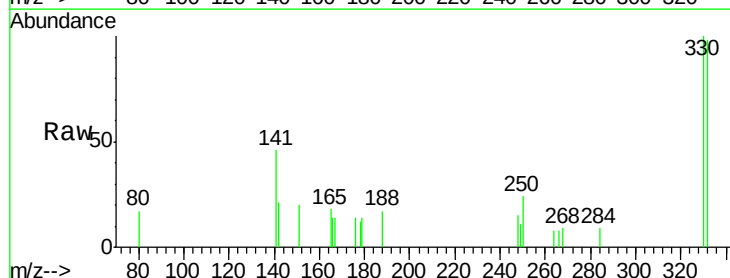


Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

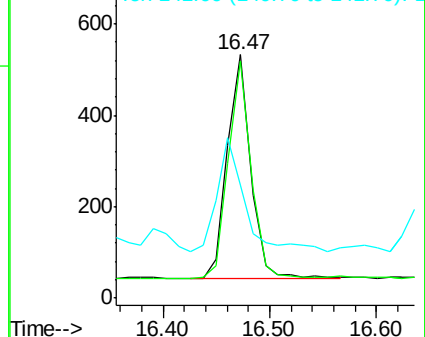

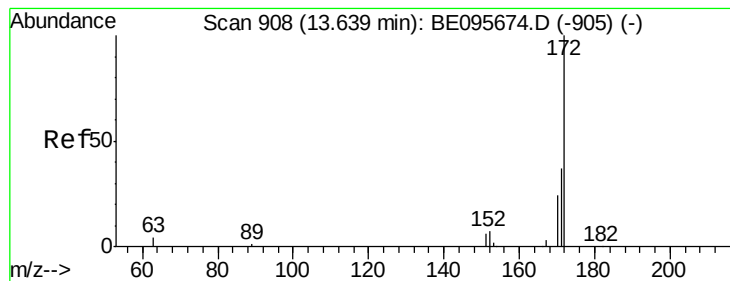

#15

2-Fluorobiphenyl

Concen: 0.336 ng

RT: 13.64 min Scan# 1168

Delta R.T. 0.00 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14

Instrument :

BNA_E

ClientSampleId :

CPS093071


Tot Ion:172 Resp: 6909

Ion Ratio Lower Upper

172 100

171 34.6 29.9 44.9




170 23.3 21.8 32.8

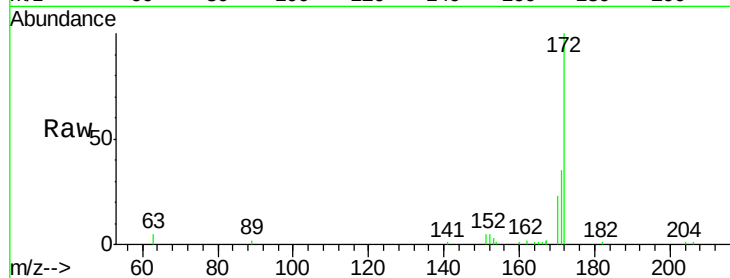

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

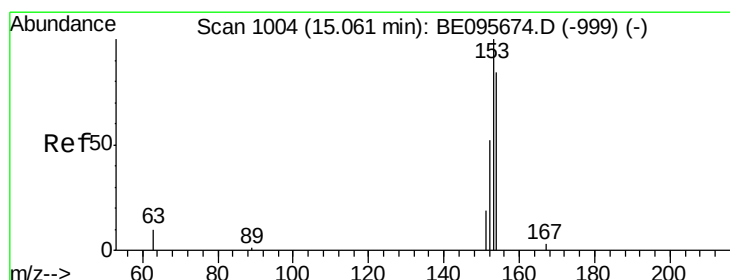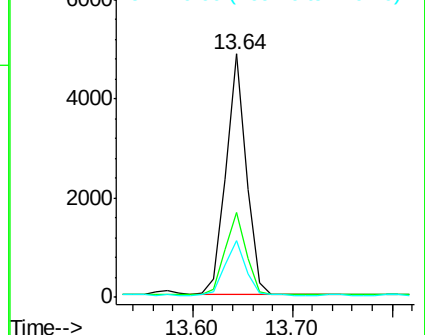

#17

Acenaphthene

Concen: 0.133 ng

RT: 15.06 min Scan# 1291

Delta R.T. -0.00 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14


Tgt Ion:154 Resp: 2163

Ion Ratio Lower Upper

154 100

153 147.3 89.2 133.8#



152 99.1 42.0 63.0#

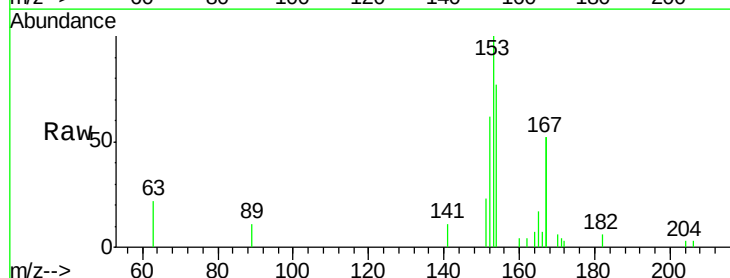


Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

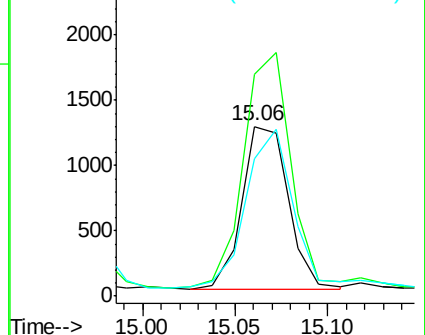



#18

Fluorene

Concen: 0.225 ng

RT: 16.03 min Scan# 1371

Delta R.T. 0.00 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14

Instrument :

BNA_E

ClientSampleId :

CPS093071





Tot Ion:166 Resp: 4532

Ion Ratio Lower Upper

166 100

165 103.7 77.8 116.6

167 24.3 42.4 63.6#

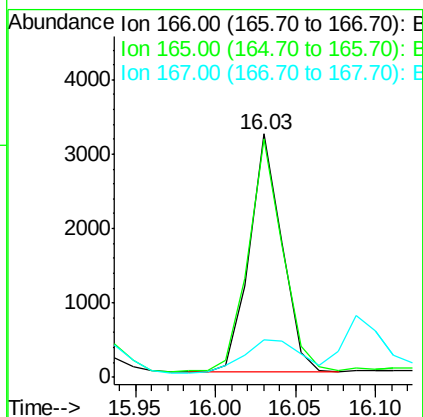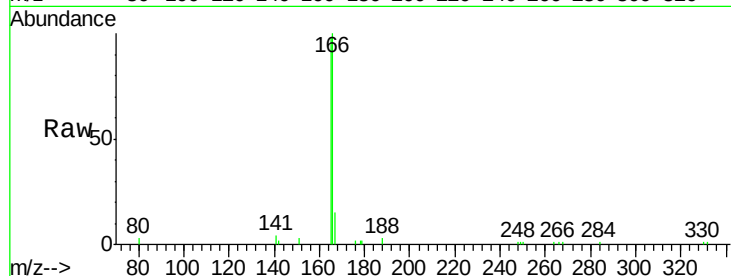

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.71 min Scan# 1515

Delta R.T. 0.01 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14




Tgt Ion:188 Resp: 8631


Ion Ratio Lower Upper

188 100

94 0.0 3.9 5.9#

80 12.6 3.6 5.4#

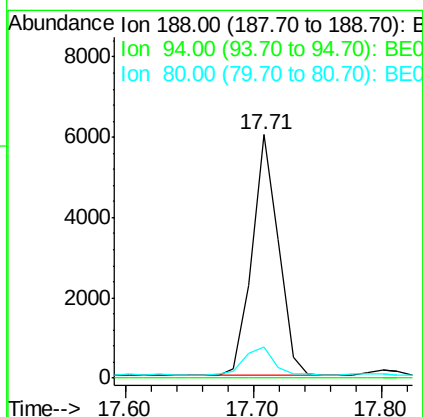



#22

Pentachlorophenol

Concen: 175.119 ng

RT: 17.37 min Scan# 1486

Delta R.T. -0.00 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14

Instrument :

BNA_E

ClientSampleId :

CPS093071


Tot Ion:266 Resp: 360391

Ion Ratio Lower Upper

266 100

264 61.1 72.5 108.7#




268 65.7 73.8 110.6#

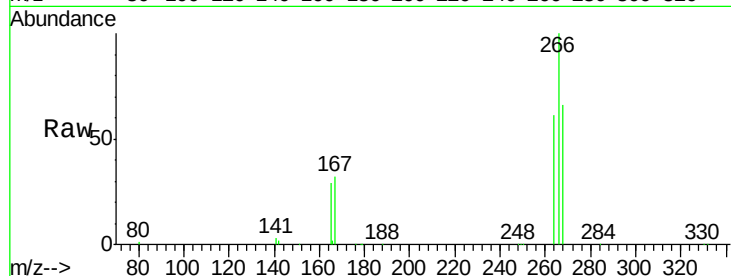

Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

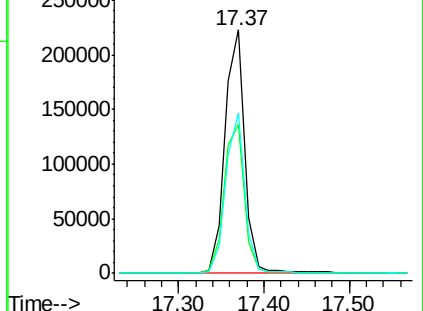

#23

Phenanthrene

Concen: 0.055 ng

RT: 17.75 min Scan# 1519

Delta R.T. 0.01 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14


Tgt Ion:178 Resp: 1481

Ion Ratio Lower Upper

178 100

176 20.2 15.1 22.7



179 17.4 11.8 17.6




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E




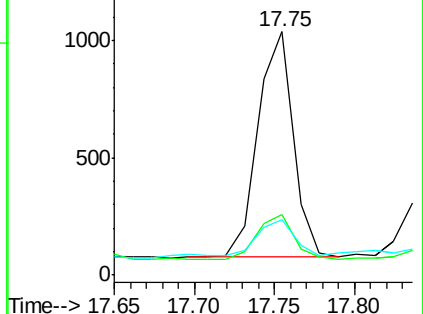


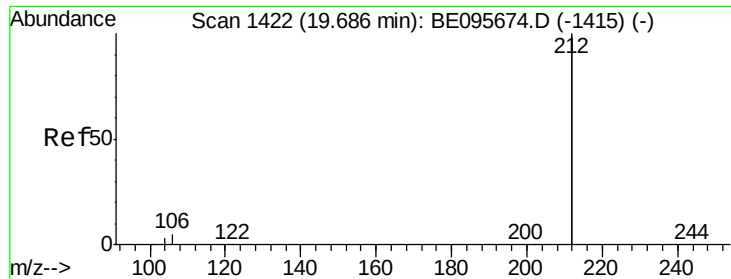

#25
 Fluoranthene-d10
 Concen: 0.378 ng
 RT: 19.69 min Scan# 1829
 Delta R.T. 0.00 min
 Lab File: BE095727.D
 Acq: 12 Mar 2018 13:14




Instrument :
 BNA_E
 ClientSampleId :
 CPS093071


Tot Ion:212 Resp: 42669
 Ion Ratio Lower Upper
 212 100
 106 2.9 2.8 4.2
 104 1.8 1.6 2.4

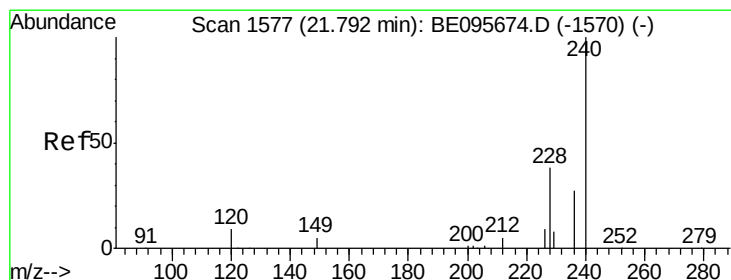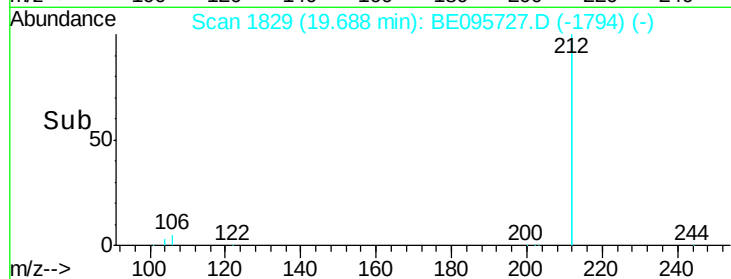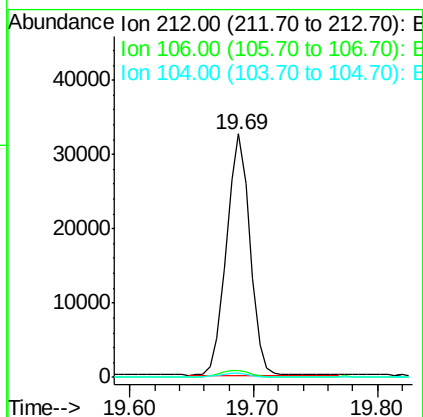

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.80 min Scan# 2029
 Delta R.T. 0.01 min
 Lab File: BE095727.D
 Acq: 12 Mar 2018 13:14

Tgt Ion:240 Resp: 8722
 Ion Ratio Lower Upper
 240 100
 120 7.1 5.5 8.3
 236 27.5 20.7 31.1

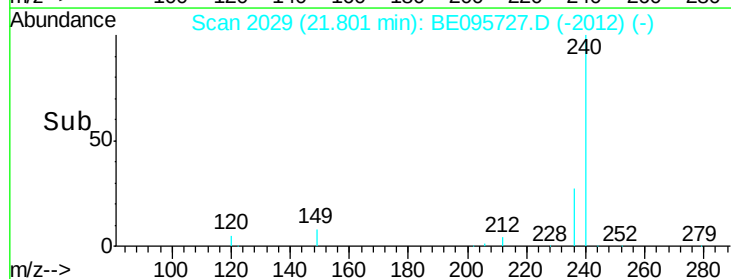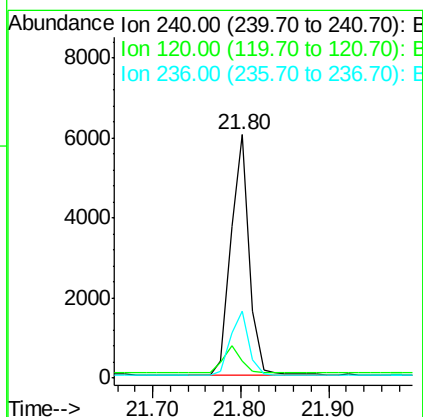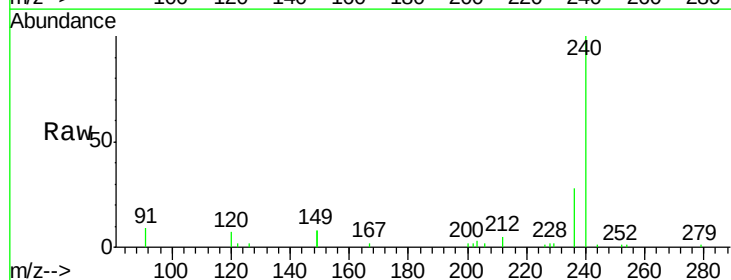

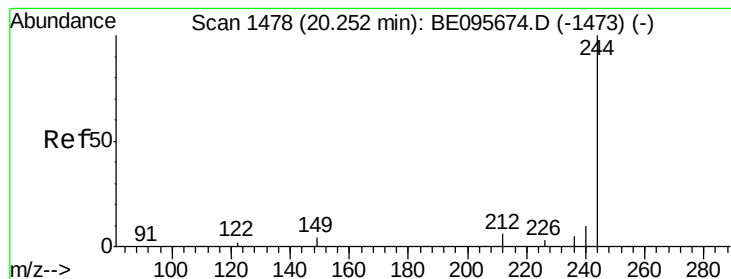

#29

Terphenyl-d14

Concen: 0.394 ng

RT: 20.25 min Scan# 1901

Delta R.T. 0.00 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14

Instrument :

BNA_E

ClientSampleId :

CPS093071


Tot Ion:244 Resp: 6853

Ion Ratio Lower Upper

244 100

212 7.6 25.4 38.0#




122 5.6 8.1 12.1#

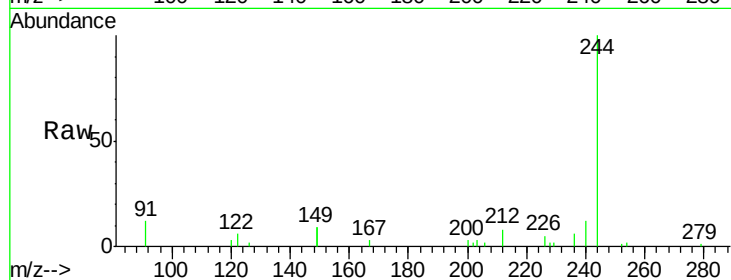

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

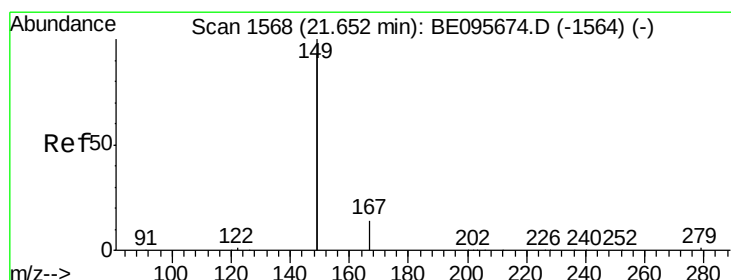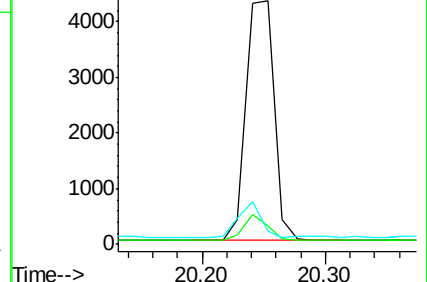

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.155 ng

RT: 21.66 min Scan# 2017

Delta R.T. 0.00 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14


Tgt Ion:149 Resp: 7786

Ion Ratio Lower Upper

149 100

167 7.6 5.4 8.0



279 0.8 0.7 1.1



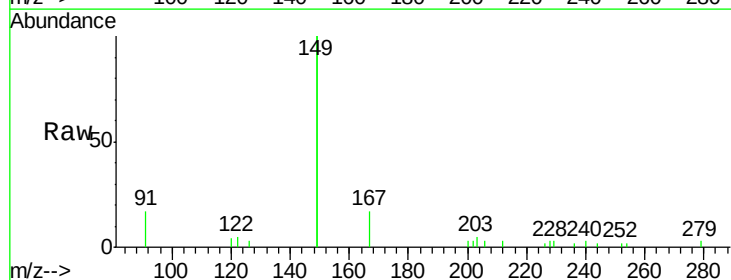


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

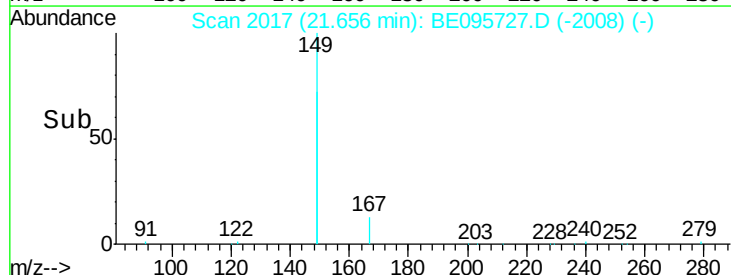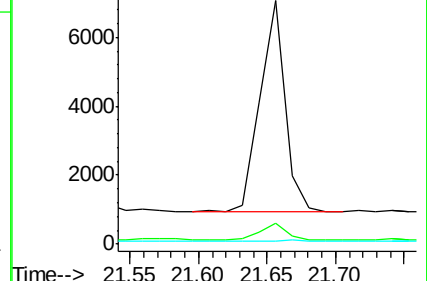

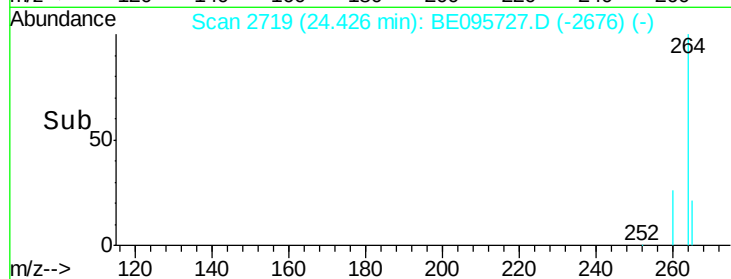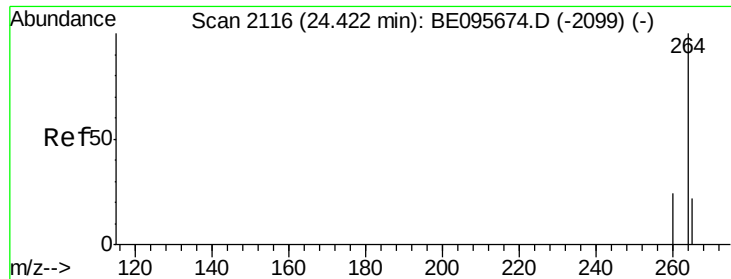

#34

Pervlone-d12

Concen: 0.400 ng

RT: 24.43 min Scan# 2719

Delta R.T. 0.00 min

Lab File: BE095727.D

Acq: 12 Mar 2018 13:14

Instrument :

BNA_E

ClientSampleId :

CPS093071

Tot Ion:264 Resp: 8194

Ion Ratio Lower Upper

264 100

260 26.7 20.5 30.7

265 25.6 22.8 34.2

