


Data Path : Z:\HPCHEM1\BNA_E\Data\BE031218\
Data File : BE095722.D
Acq On : 12 Mar 2018 8:28
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE031318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 13 17:41:41 2018

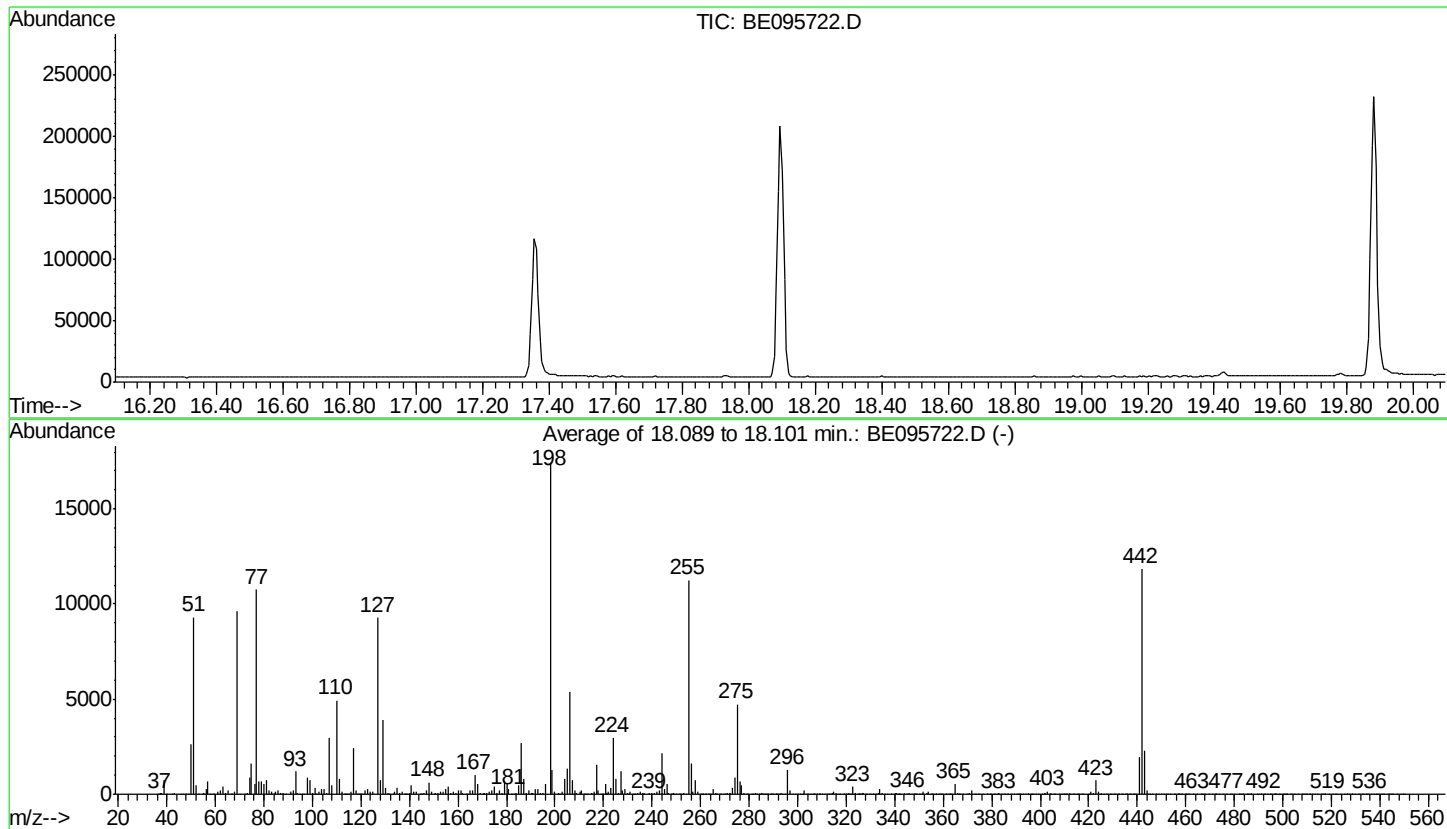

AutoFind: Scans 2638, 2639, 2640; Background Corrected with Scan 2627

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	53.3	9290	PASS
68	69	0.00	2	1.7	160	PASS
69	198	0.00	100	55.2	9630	PASS
70	69	0.00	2	0.3	33	PASS
127	198	10	80	53.2	9279	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17437	PASS
199	198	5	9	7.4	1282	PASS
275	198	10	60	27.1	4734	PASS
365	198	1	100	3.2	553	PASS
441	443	0.01	100	83.6	1935	PASS
442	198	50	100	68.0	11857	PASS
443	442	15	24	19.5	2315	PASS