


Data Path : Z:\HPCHEM1\BNA_E\Data\BE031218\
Data File : BE095739.D
Acq On : 12 Mar 2018 21:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE031318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 13 17:41:41 2018

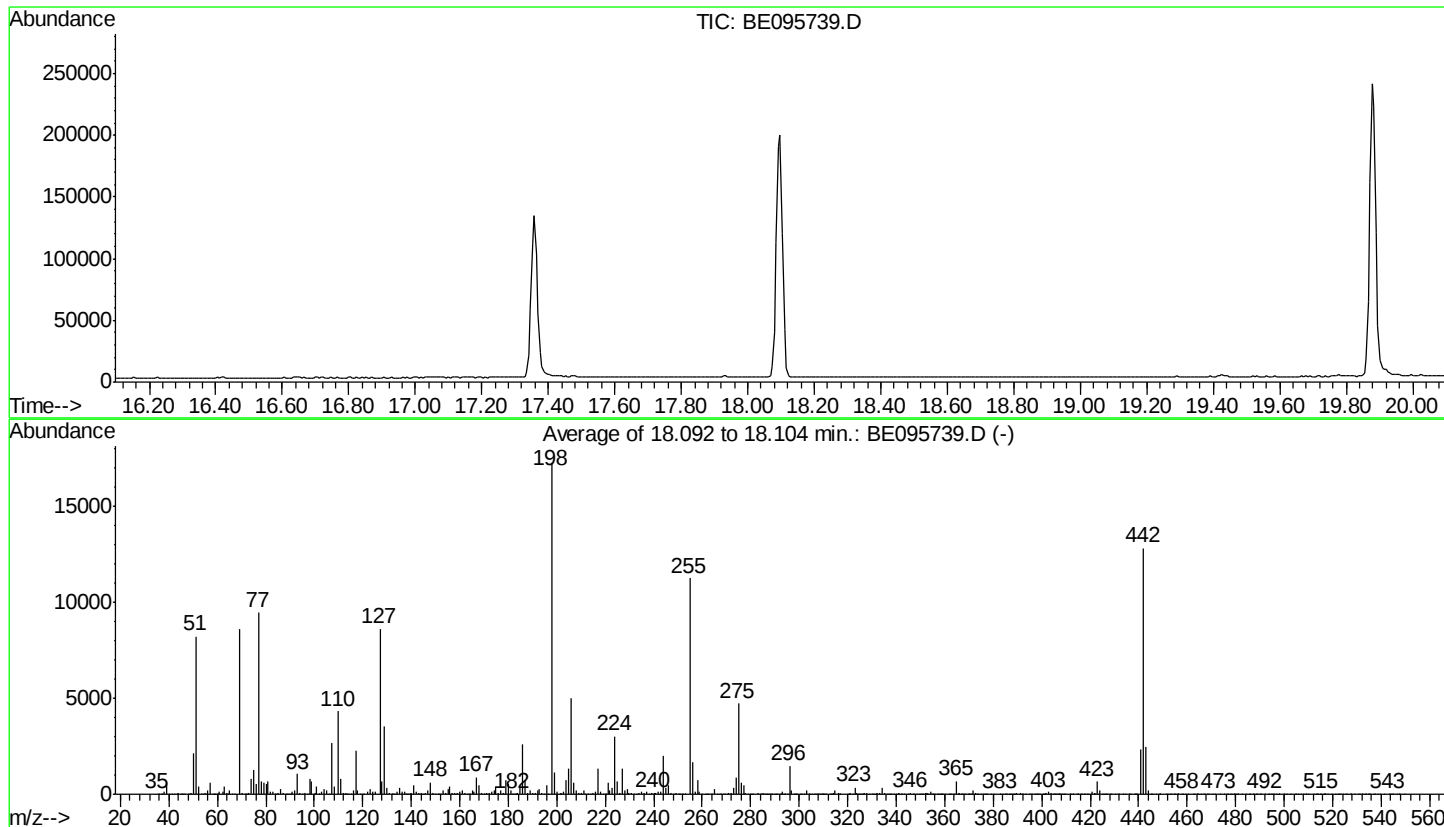

AutoFind: Scans 2639, 2640, 2641; Background Corrected with Scan 2632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.6	8234	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.7	8590	PASS
70	69	0.00	2	0.6	50	PASS
127	198	10	80	49.9	8627	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17282	PASS
199	198	5	9	6.7	1151	PASS
275	198	10	60	27.3	4716	PASS
365	198	1	100	4.0	685	PASS
441	443	0.01	100	95.3	2325	PASS
442	198	50	100	74.3	12832	PASS
443	442	15	24	19.0	2439	PASS