

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031319\
 Data File : BE098913.D
 Acq On : 13 Mar 2019 15:55
 Operator : JU/SJ
 Sample : K1841-09DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Mar 14 06:55:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 06 15:33:24 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	641	0.40	ng	0.01
7) Naphthalene-d8	10.61	136	3148	0.40	ng	0.02
13) Acenaphthene-d10	14.47	164	2516	0.40	ng	0.02
19) Phenanthrene-d10	17.21	188	6157	0.40	ng	0.00
27) Chrysene-d12	21.40	240	6654	0.40	ng	0.00
34) Perylene-d12	23.90	264	6452	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.42	112	38	0.02	ng	0.04
5) Phenol-d6	7.01	99	2	0.00	ng	0.03
8) Nitrobenzene-d5	8.99	82	13	0.00	ng	0.02
11) 2-Methylnaphthalene-d10	12.24	152	436	0.07	ng	0.04
14) 2,4,6-Tribromophenol	16.00	330	61	0.05	ng	0.03
15) 2-Fluorobiphenyl	13.13	172	838	0.08	ng	0.04
25) Fluoranthene-d10	19.26	212	7259	0.07	ng	0.02
29) Terphenyl-d14	19.86	244	1529	0.09	ng	0.01
Target Compounds						
2) 1,4-Dioxane	3.28	88	2627	2.558	ng	96
3) n-Nitrosodimethylamine	3.63	42	46	0.029	ng	# 46
22) Pentachlorophenol	16.84	266	11	0.273	ng	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031319\
Data File : BE098913.D
Acq On : 13 Mar 2019 15:55
Operator : JU/SJ
Sample : K1841-09DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Mar 14 06:55:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 15:33:24 2019
Response via : Initial Calibration

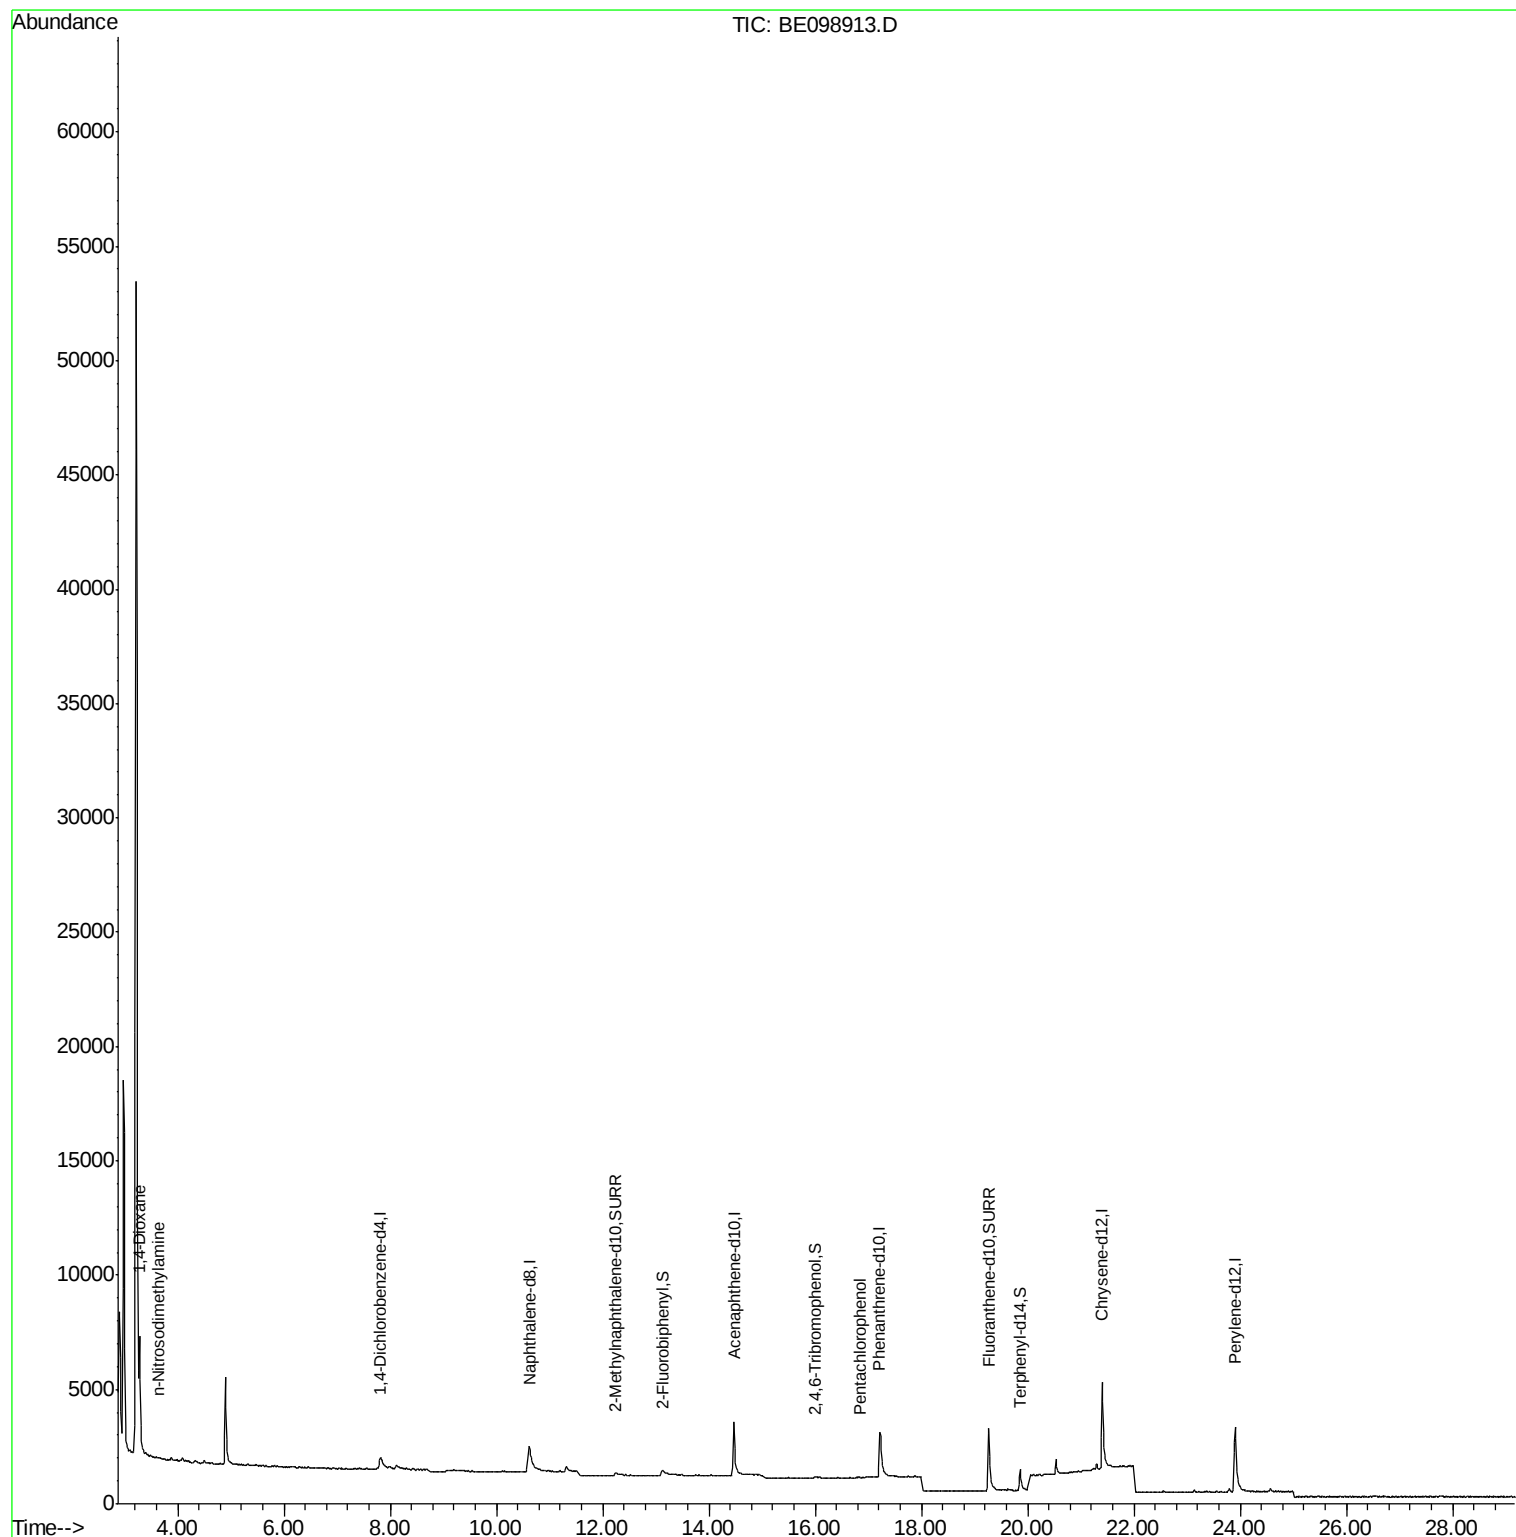




#1



1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.81 min Scan# 429
Delta R.T. 0.01 min
Lab File: BE098913.D
Acq: 13 Mar 2019 15:55

Instrument :
BNA_E
ClientSampled :

Tot Ion:152 Resp: 641
Ion Ratio Lower Upper
152 100
150 147.0 122.5 183.7
115 82.5 57.4 86.2

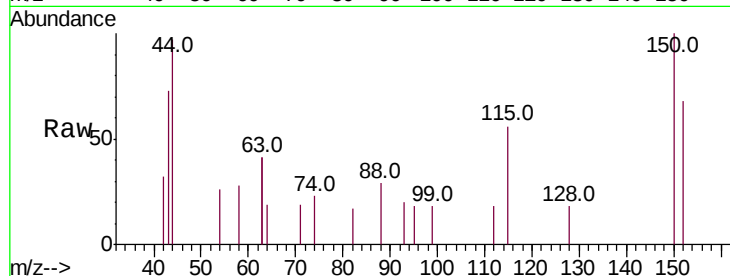


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

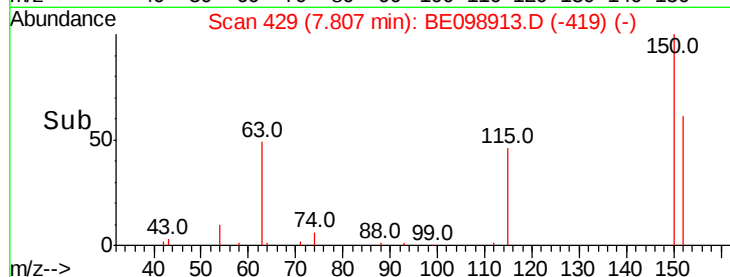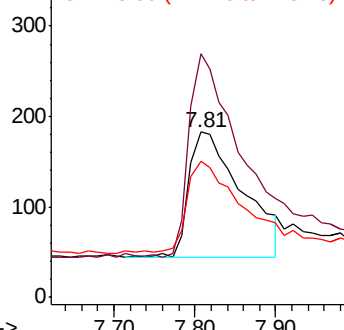



#2

1,4-Dioxane
Concen: 2.558 ng
RT: 3.28 min Scan# 36
Delta R.T. -0.01 min
Lab File: BE098913.D
Acq: 13 Mar 2019 15:55

Tgt Ion: 88 Resp: 2627
Ion Ratio Lower Upper
88 100
58 99.0 75.8 113.6
43 49.8 41.8 62.8

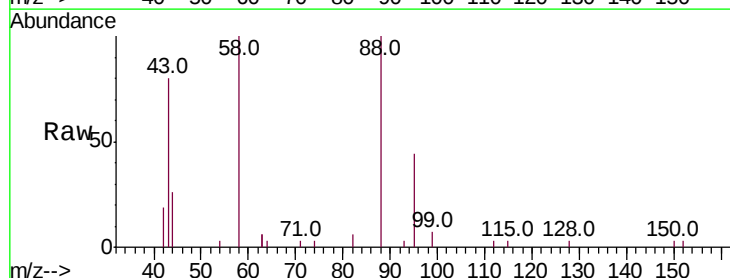

Abundance Ion 88.00 (87.70 to 88.70): BE0
Ion 58.00 (57.70 to 58.70): BE0
Ion 43.00 (42.70 to 43.70): BE0

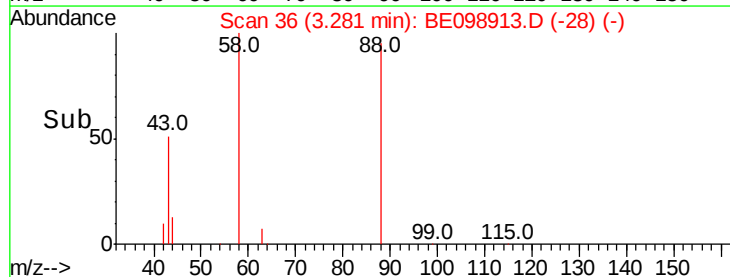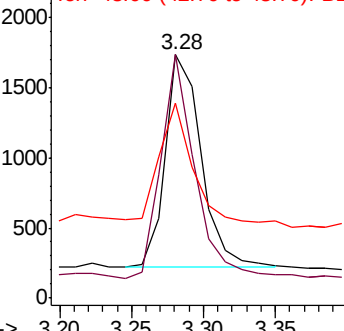



#3

n-Nitrosodimethylamine

Concen: 0.029 ng

RT: 3.63 min Scan# 66

Delta R.T. 0.00 min

Lab File: BE098913.D


Acq: 13 Mar 2019 15:55

Instrument :

BNA_E

ClientSampleId :




Tot Ion:	42	Resp:	46
Ion	Ratio	Lower	Upper
42	100		
74	26.1	57.0	85.4#
44	0.0	0.0	0.0

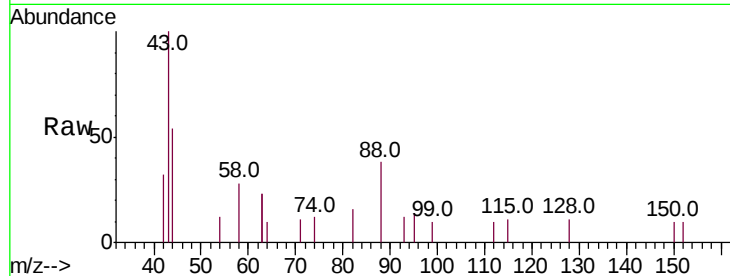

Abundance Ion 42.00 (41.70 to 42.70): BE0

Ion 74.00 (73.70 to 74.70): BE0

Ion 44.00 (43.70 to 44.70): BE0

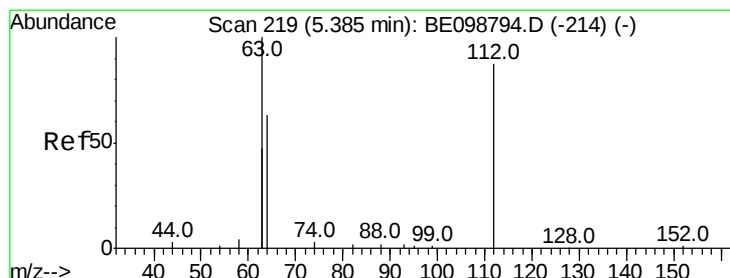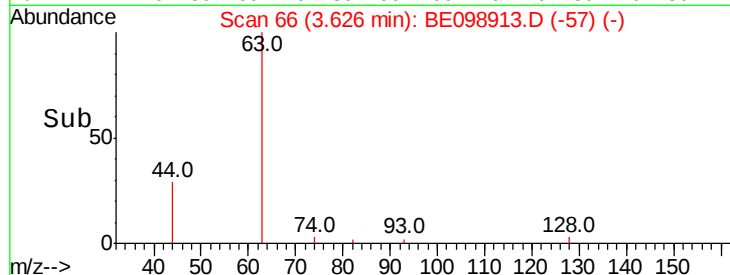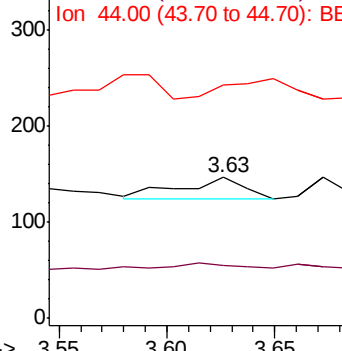

#4

2-Fluorophenol

Concen: 0.020 ng


RT: 5.42 min Scan# 222

Delta R.T. 0.04 min

Lab File: BE098913.D

Acq: 13 Mar 2019 15:55



Tgt Ion:	112	Resp:	38
Ion	Ratio	Lower	Upper
112	100		
64	26.3	57.9	86.9#
63	0.0	158.3	237.5#

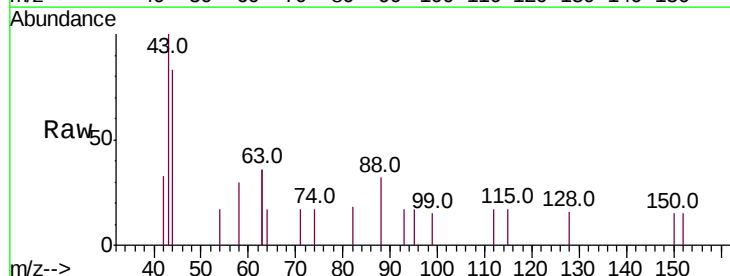


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BE0

Ion 63.00 (62.70 to 63.70): BE0

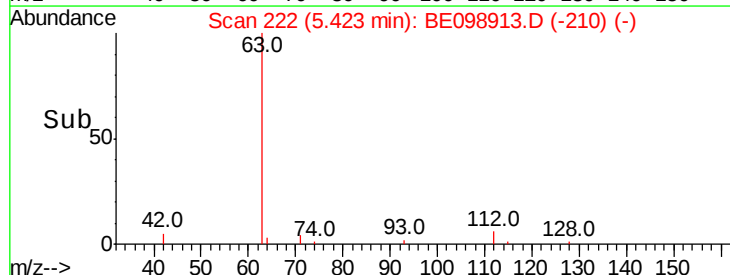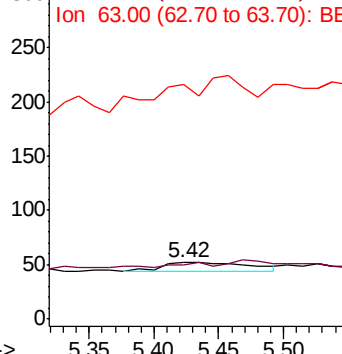



#5

Phenol-d6

Concen: 0.001 ng

RT: 7.01 min Scan# 360

Delta R.T. 0.03 min

Lab File: BE098913.D





Acq: 13 Mar 2019 15:55

Instrument :

BNA_E

ClientSampleId :

Tot Ion:	99	Resp:	2
Ion	Ratio	Lower	Upper
99	100		
42	850.0	24.2	36.2#
71	300.0	35.7	53.5#

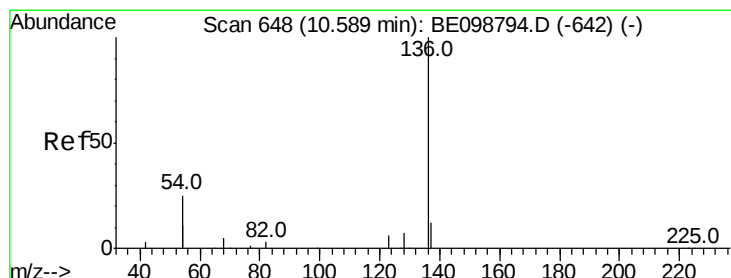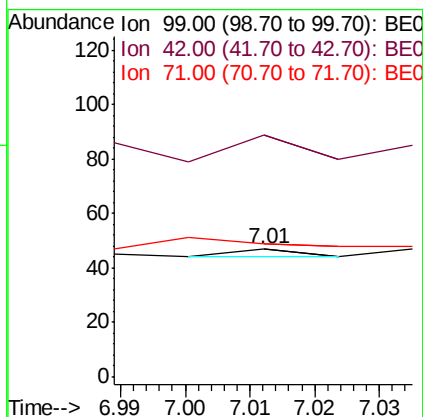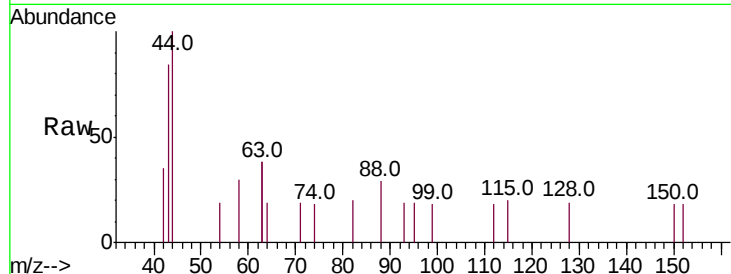

#7

Naphthalene-d8

Concen: 0.400 ng




RT: 10.61 min Scan# 650


Delta R.T. 0.02 min

Lab File: BE098913.D

Acq: 13 Mar 2019 15:55

Tgt Ion:	136	Resp:	3148
Ion	Ratio	Lower	Upper
136	100		
137	18.5	11.4	17.0#
54	70.3	39.3	58.9#
68	13.1	6.7	10.1#

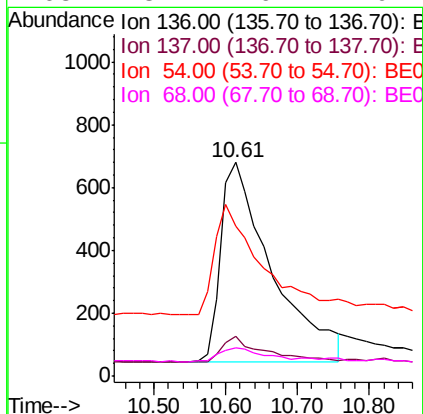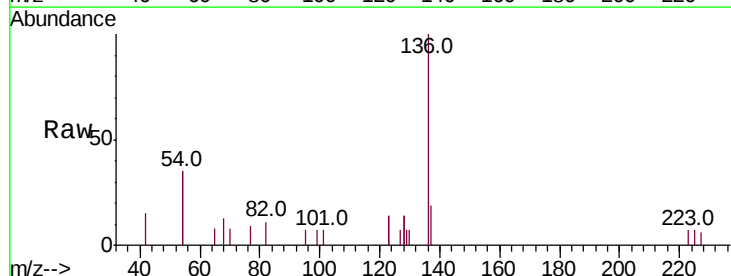



#8

Nitrobenzene-d5

Concen: 0.004 ng

RT: 8.99 min Scan# 525

Delta R.T. 0.02 min

Lab File: BE098913.D

Acq: 13 Mar 2019 15:55

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 82 Resp: 13

Ion Ratio Lower Upper




82 100

128 359.3 123.8 185.8#

54 366.7 203.4 305.2#

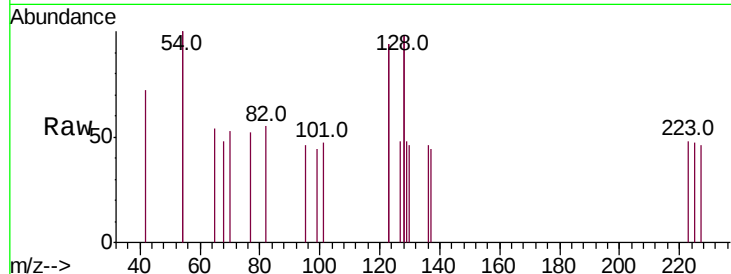

Abundance Ion 82.00 (81.70 to 82.70): BE098794.D (-517) (-)

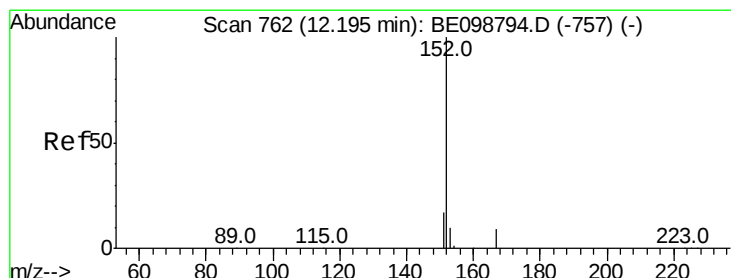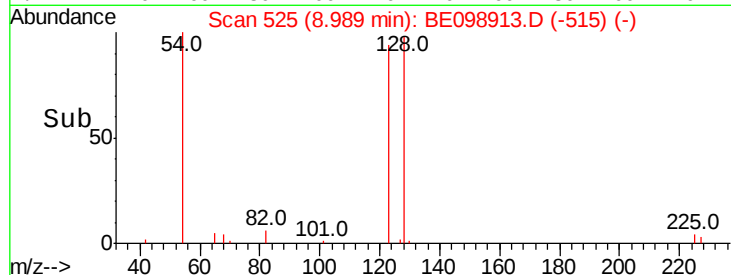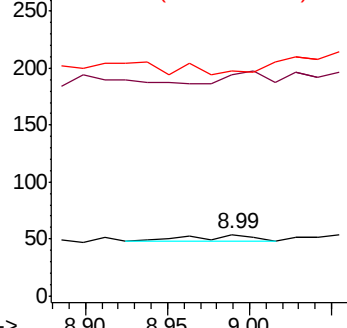

#11

2-Methylnaphthalene-d10

Concen: 0.075 ng

RT: 12.24 min Scan# 765

Delta R.T. 0.04 min

Lab File: BE098913.D


Acq: 13 Mar 2019 15:55

Tgt Ion: 152 Resp: 436



Ion Ratio Lower Upper


152 100

151 14.9 16.5 24.7#

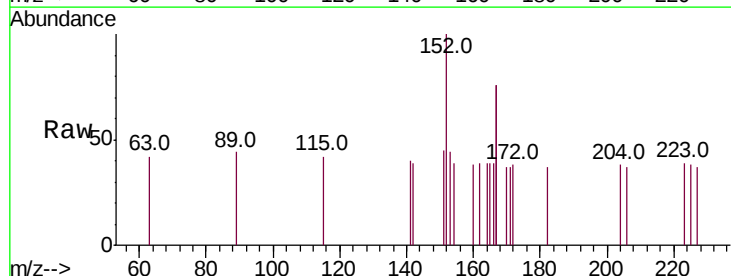

Abundance Ion 152.00 (151.70 to 152.70): BE098794.D (-757) (-)

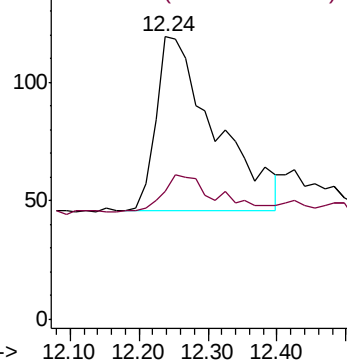







#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.47 min Scan# 920
 Delta R.T. 0.02 min
 Lab File: BE098913.D
 Acq: 13 Mar 2019 15:55

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:164 Resp: 2516
 Ion Ratio Lower Upper
 164 100
 162 101.7 80.2 120.2
 160 50.6 37.8 56.8

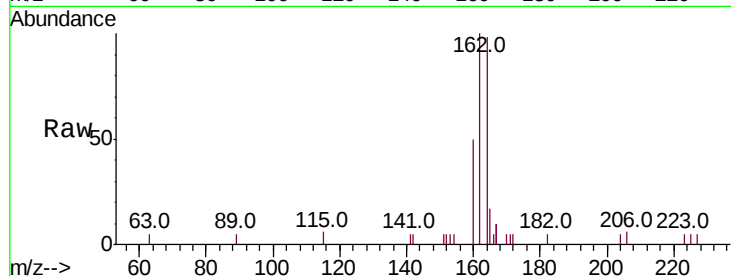


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

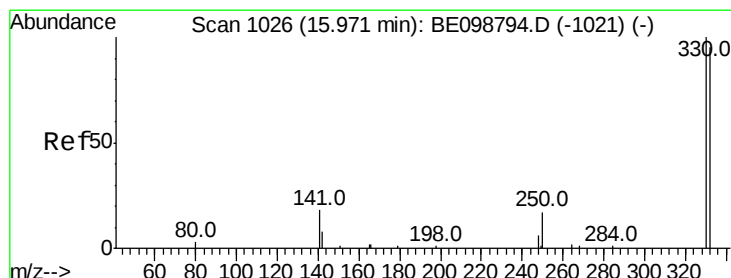
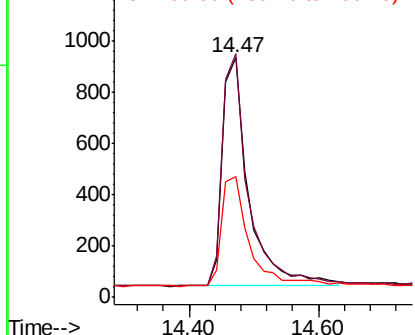



#14
 2,4,6-Tribromophenol
 Concen: 0.048 ng
 RT: 16.00 min Scan# 1028
 Delta R.T. 0.03 min
 Lab File: BE098913.D
 Acq: 13 Mar 2019 15:55

Tgt Ion:330 Resp: 61
 Ion Ratio Lower Upper
 330 100
 332 67.2 77.6 116.4#
 141 57.4 31.0 46.4#

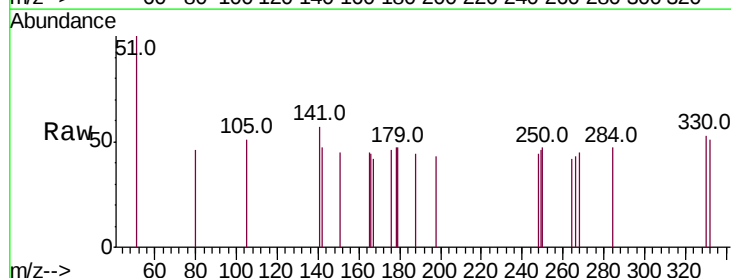

Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

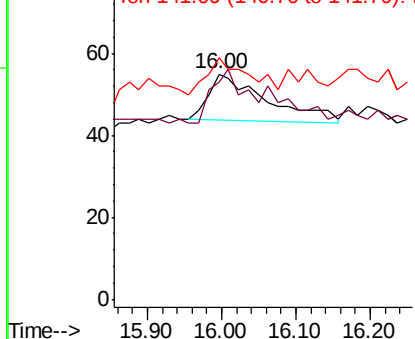


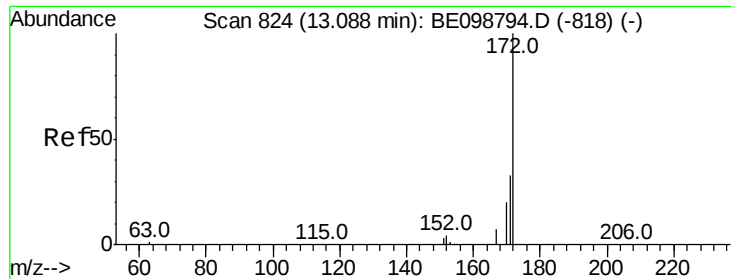




#15
2-Fluorobiphenyl
Concen: 0.080 ng
RT: 13.13 min Scan# 827
Delta R.T. 0.04 min
Lab File: BE098913.D
Acq: 13 Mar 2019 15:55

Instrument :
BNA_E
ClientSampled :

Tot Ion:172 Resp: 838
Ion Ratio Lower Upper
172 100
171 53.8 28.0 42.0#
170 39.9 17.7 26.5#

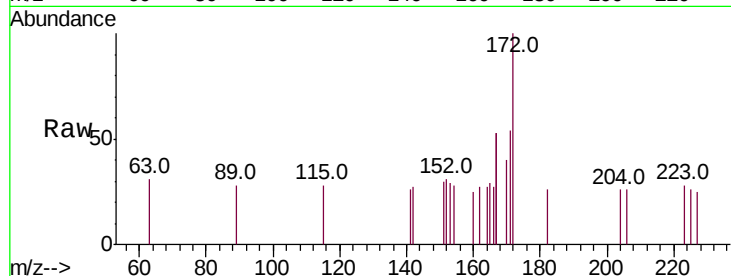


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

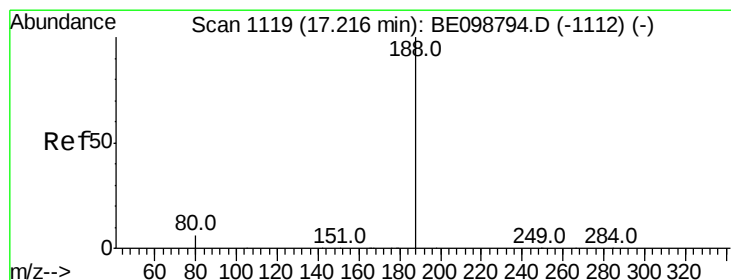
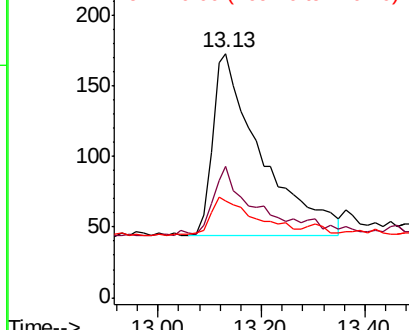



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.21 min Scan# 1119
Delta R.T. -0.00 min
Lab File: BE098913.D
Acq: 13 Mar 2019 15:55

Tgt Ion:188 Resp: 6157
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 14.0 6.3 9.5#

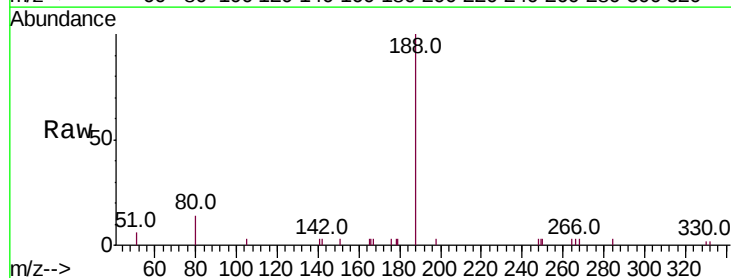

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0

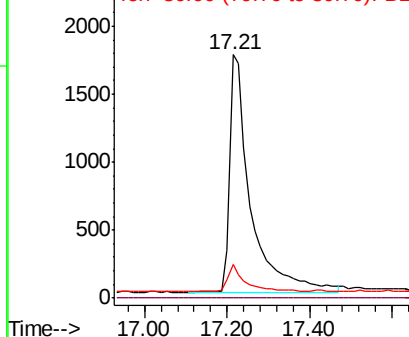

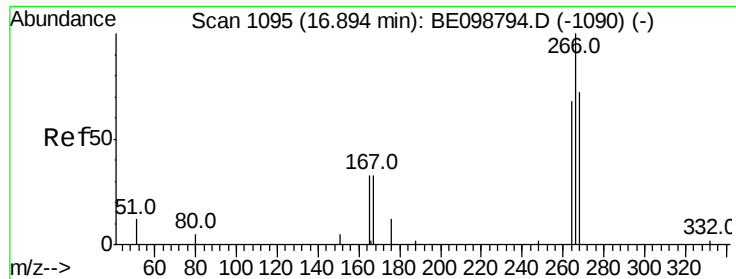

#22

Pentachlorophenol

Concen: 0.273 ng

RT: 16.84 min Scan# 1091

Delta R.T. -0.05 min

Lab File: BE098913.D

Acq: 13 Mar 2019 15:55

Instrument :

BNA_E

ClientSampled :


Tot Ion:266 Resp: 11

Ion Ratio Lower Upper

266 100

264 93.6 66.6 100.0




268 102.1 69.8 104.8

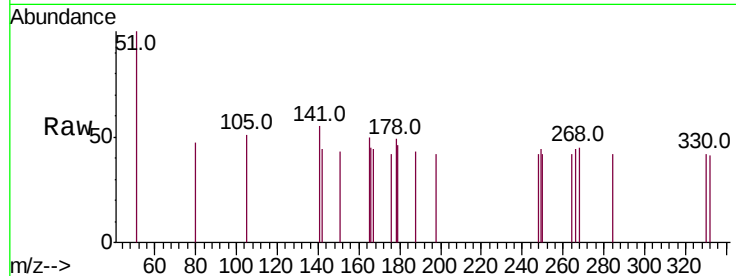

Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

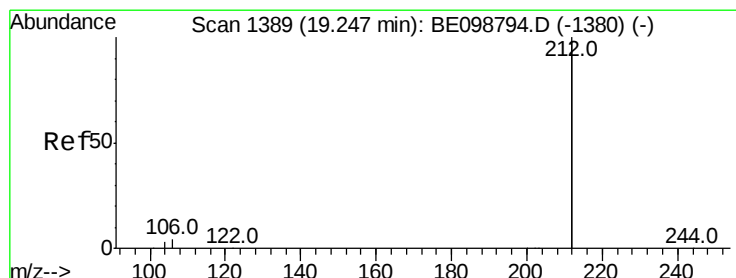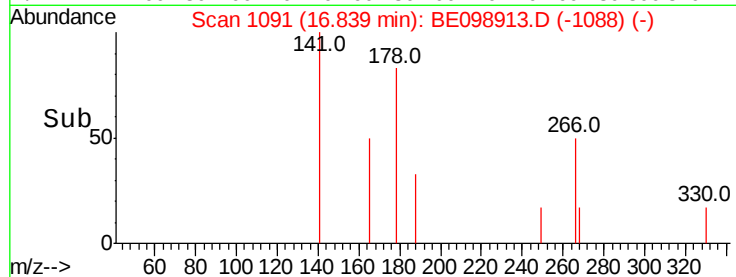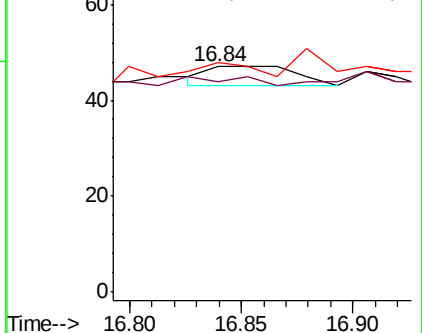

#25

Fluoranthene-d10

Concen: 0.074 ng

RT: 19.26 min Scan# 1392

Delta R.T. 0.02 min

Lab File: BE098913.D

Acq: 13 Mar 2019 15:55


Tgt Ion:212 Resp: 7259

Ion Ratio Lower Upper

212 100

106 2.1 1.8 2.8



104 1.3 1.0 1.6

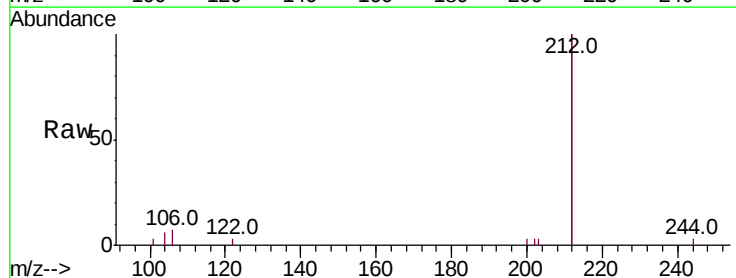


Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

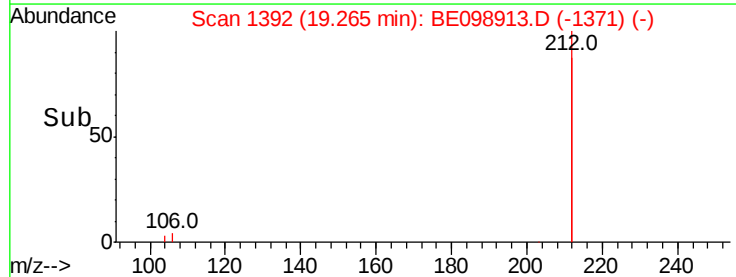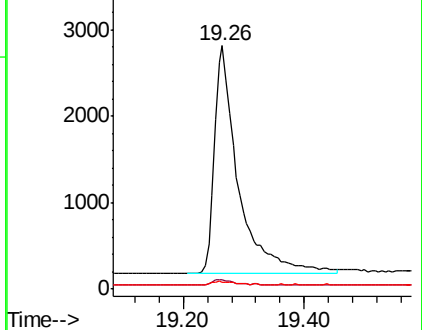



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.40 min Scan# 1633

Delta R.T. 0.00 min

Lab File: BE098913.D

Acq: 13 Mar 2019 15:55

Instrument :

BNA_E

ClientSampleId :


Tot Ion:240 Resp: 6654

Ion Ratio Lower Upper

240 100

120 9.5 5.0 7.4#




236 27.5 22.7 34.1

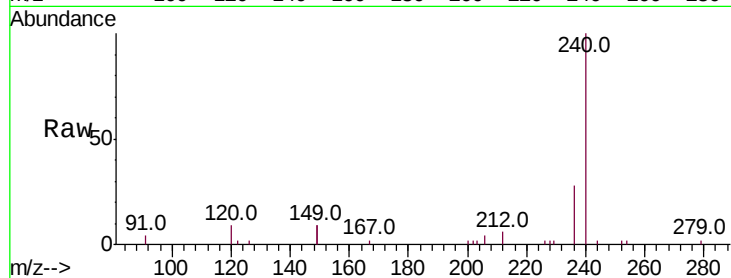

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

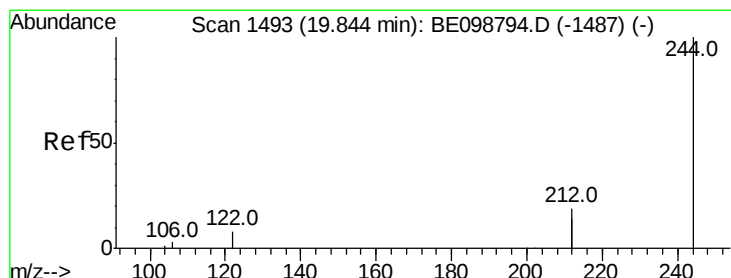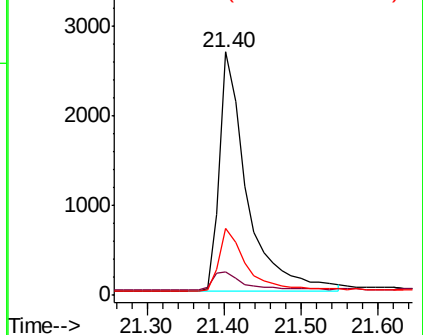

#29

Terphenyl-d14

Concen: 0.095 ng

RT: 19.86 min Scan# 1495

Delta R.T. 0.01 min

Lab File: BE098913.D

Acq: 13 Mar 2019 15:55


Tgt Ion:244 Resp: 1529

Ion Ratio Lower Upper

244 100

212 59.1 29.4 44.2#



122 13.9 7.1 10.7#


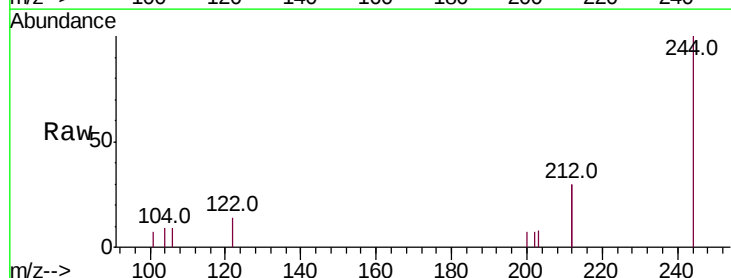


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

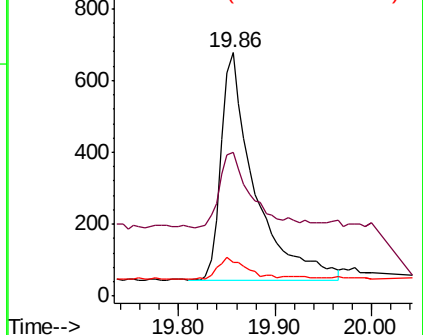

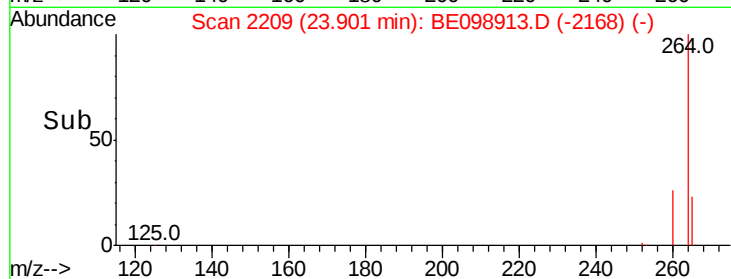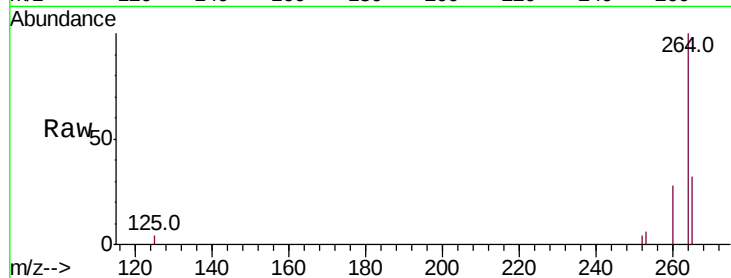

#34
Pervlene-d12
Concen: 0.400 ng
RT: 23.90 min Scan# 2209
Delta R.T. -0.00 min
Lab File: BE098913.D
Acq: 13 Mar 2019 15:55

Instrument :
BNA_E
ClientSampleId :

Tot Ion:264 Resp: 6452
Ion Ratio Lower Upper
264 100
260 27.7 21.2 31.8
265 31.6 24.6 36.8

