


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE031319\
Data File : BE098924.D
Acq On : 13 Mar 2019 23:23
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 15 18:51:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 15 05:31:33 2019
Response via : Initial Calibration

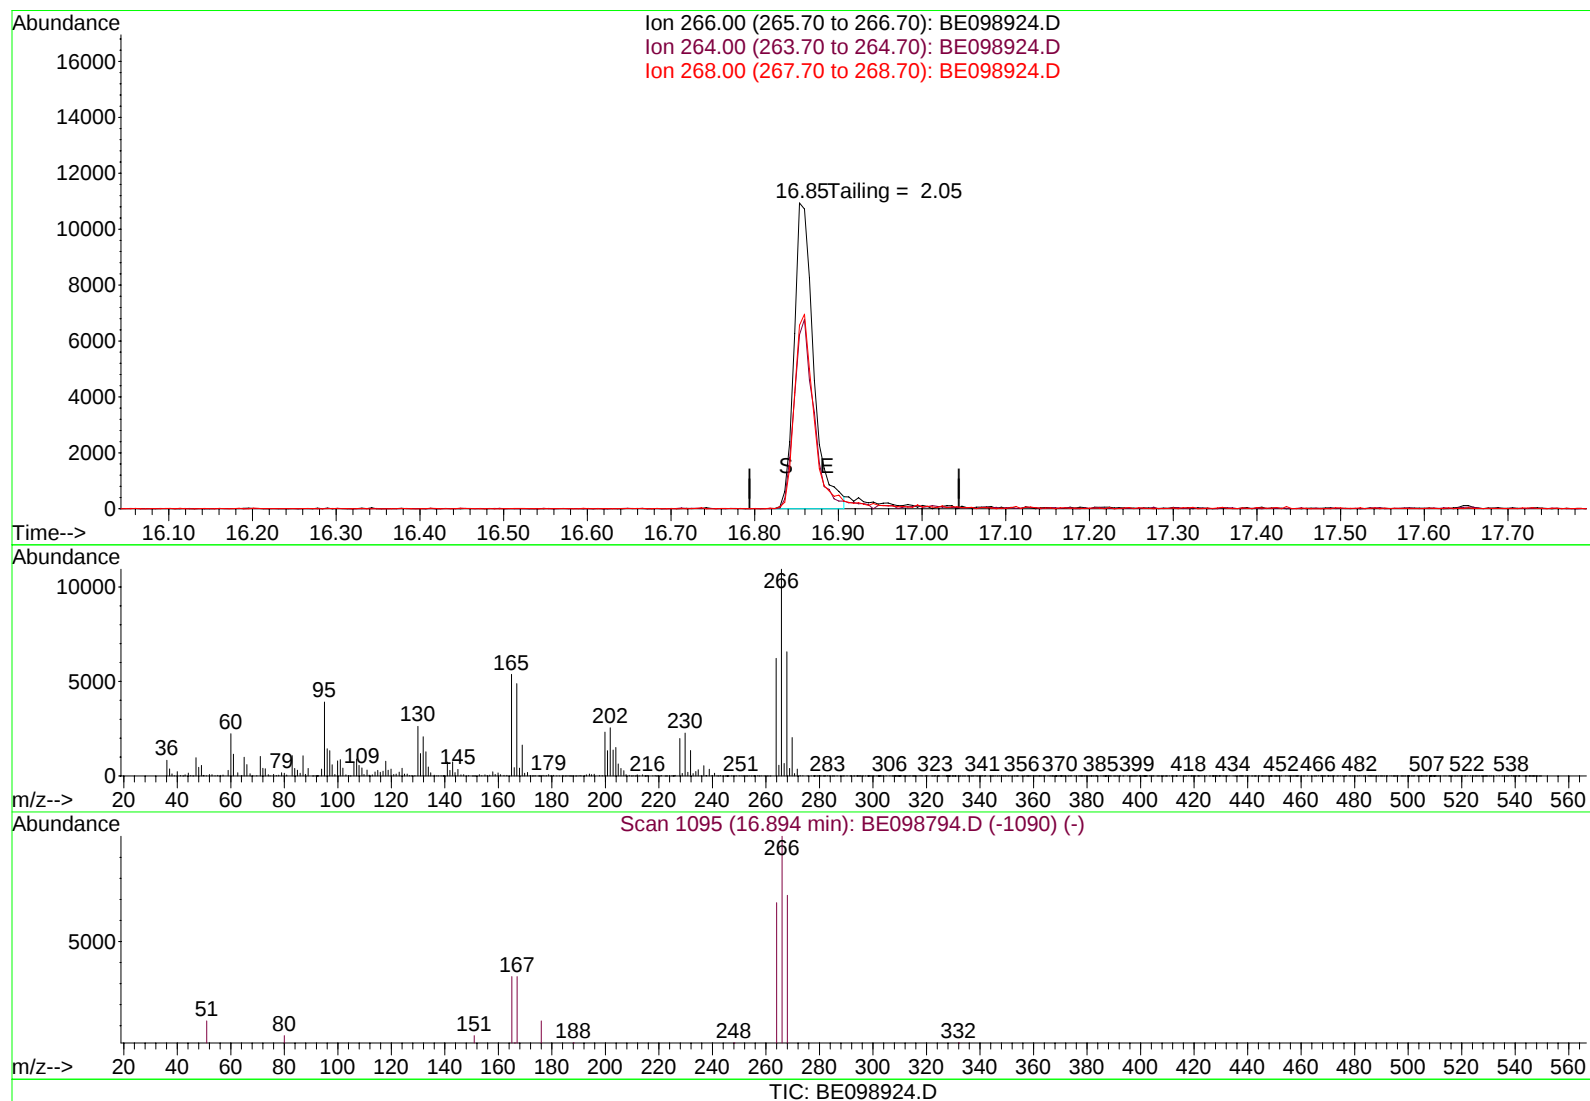

(22) Pentachlorophenol

16.854min (-0.040) 10094.86ng m

response 17720

Ion	Exp%	Act%
266.00	100	100
264.00	83.30	56.92#
268.00	87.30	60.04#
0.00	0.00	0.00