

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031319\
 Data File : BE098920.D
 Acq On : 13 Mar 2019 20:15
 Operator : JU/SJ
 Sample : K1856-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 BP-TT-AOC22-MW08-20190311

Quant Time: Mar 14 07:21:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 06 15:33:24 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	903	0.40	ng	0.00
7) Naphthalene-d8	10.59	136	3899	0.40	ng	0.00
13) Acenaphthene-d10	14.46	164	2765	0.40	ng	0.00
19) Phenanthrene-d10	17.22	188	7113	0.40	ng	0.00
27) Chrysene-d12	21.39	240	8090	0.40	ng	-0.01
34) Perylene-d12	23.89	264	7882	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.40	112	395	0.15	ng	0.01
5) Phenol-d6	6.99	99	372	0.10	ng	0.00
8) Nitrobenzene-d5	8.99	82	1377	0.34	ng	0.03
11) 2-Methylnaphthalene-d10	12.19	152	2501	0.35	ng	0.00
14) 2,4,6-Tribromophenol	15.96	330	648	0.46	ng	-0.01
15) 2-Fluorobiphenyl	13.07	172	8676	0.76	ng	-0.01
25) Fluoranthene-d10	19.24	212	34985	0.31	ng	0.00
29) Terphenyl-d14	19.84	244	9817	0.50	ng	0.00
Target Compounds						
32) Bis(2-ethylhexyl)phthalate	21.29	149	4231	0.079	ng	Qvalue # 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031319\
Data File : BE098920.D
Acq On : 13 Mar 2019 20:15
Operator : JU/SJ
Sample : K1856-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW08-20190311

Quant Time: Mar 14 07:21:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE030619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 06 15:33:24 2019
Response via : Initial Calibration

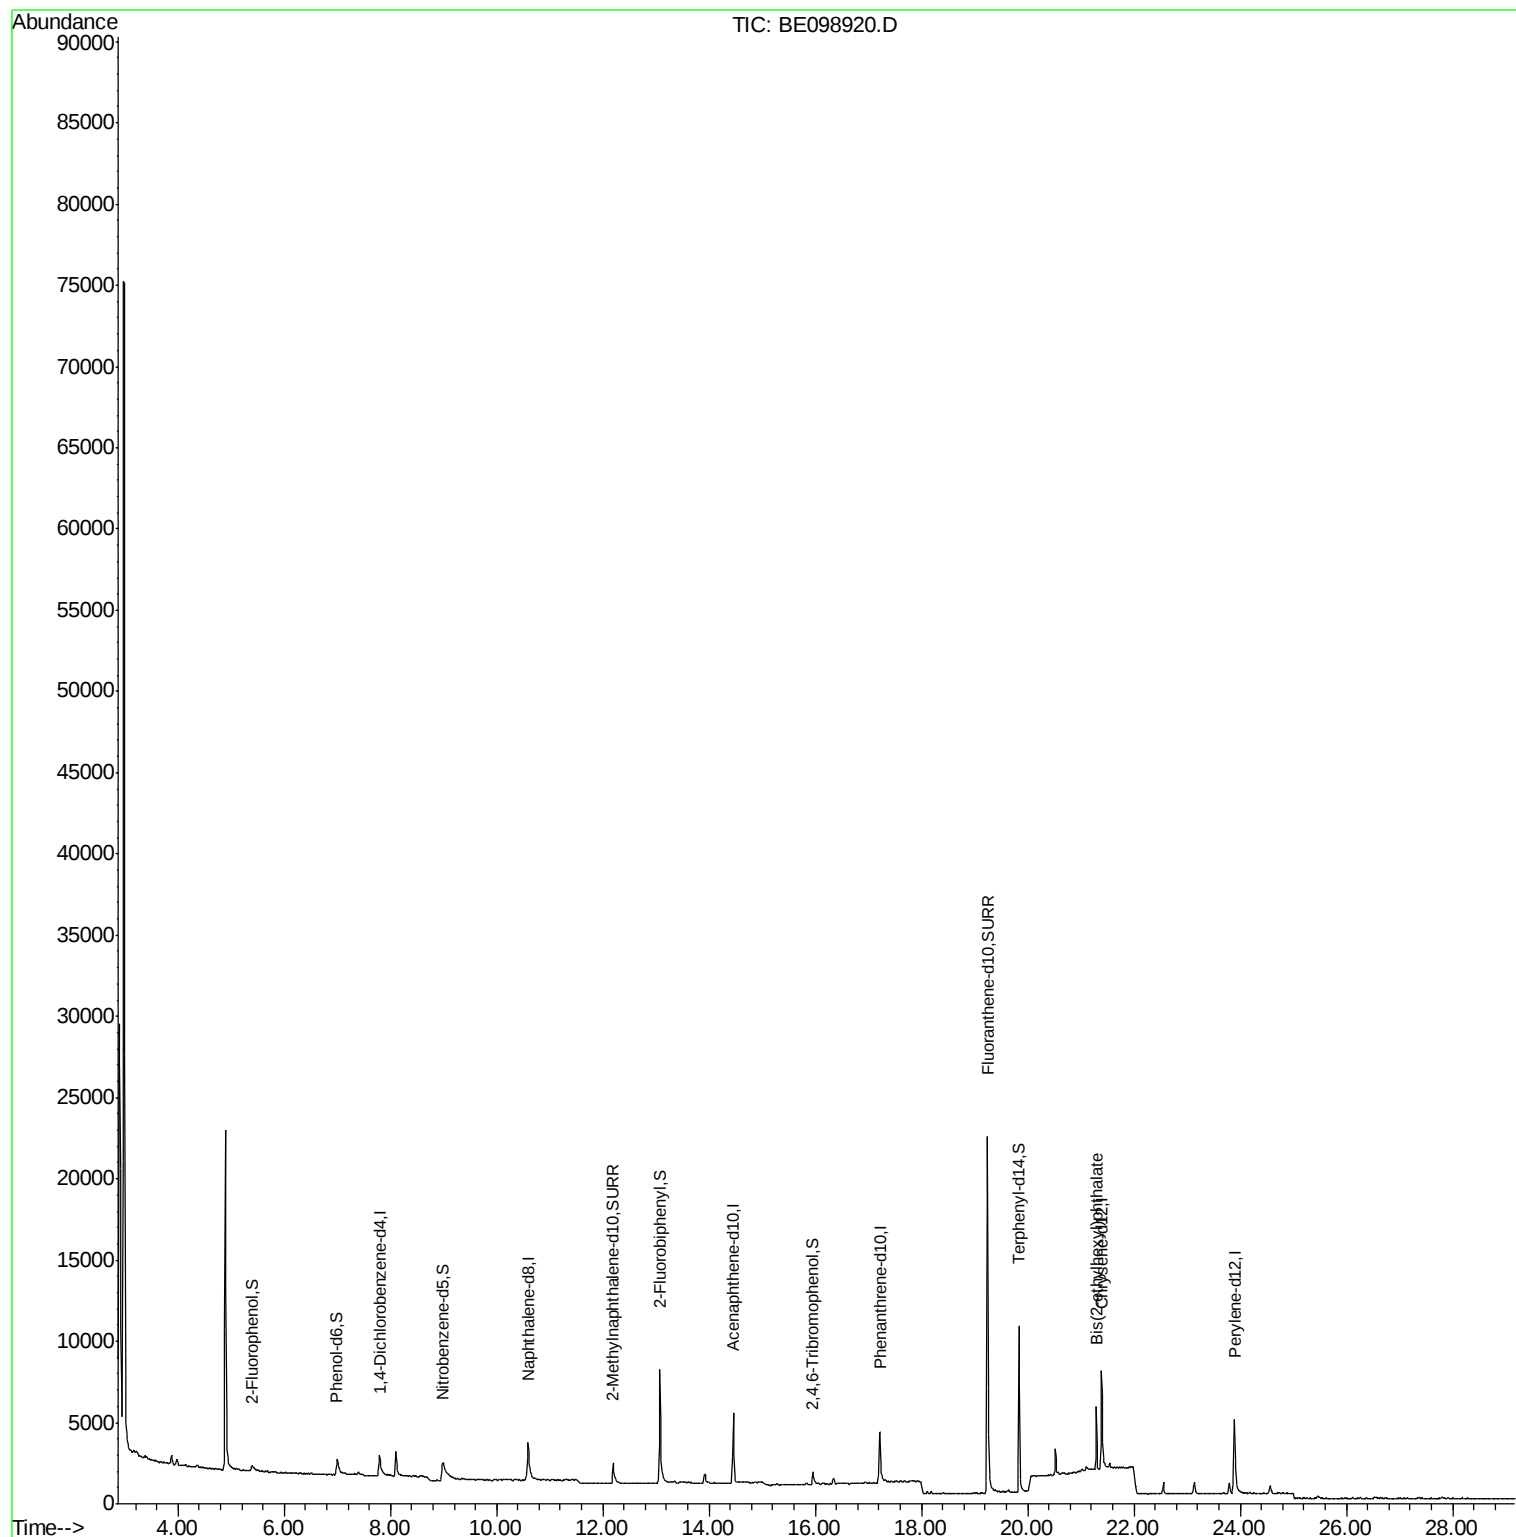




#1


1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.79 min Scan# 428
Delta R.T. -0.00 min
Lab File: BE098920.D
Acq: 13 Mar 2019 20:15

Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW08-20190311



Tot Ion:152 Resp: 903
Ion Ratio Lower Upper
152 100
150 161.4 122.5 183.7
115 80.8 57.4 86.2

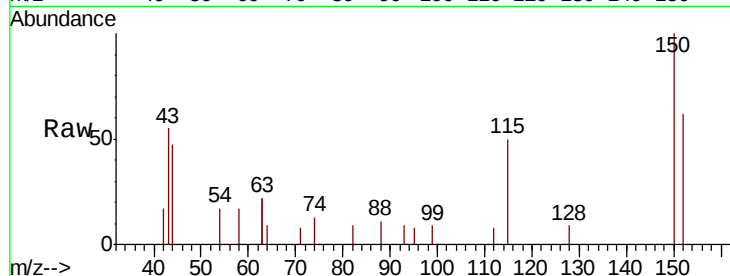

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

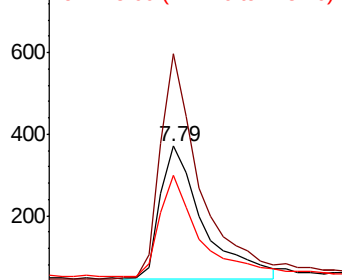


Time-->

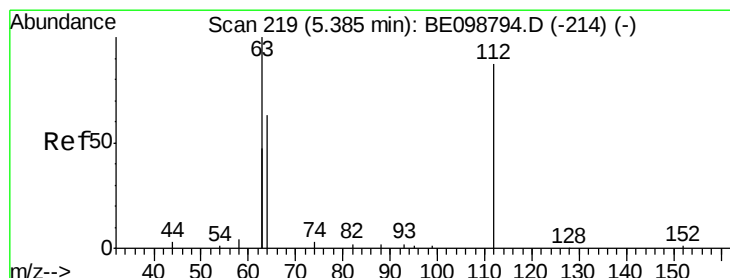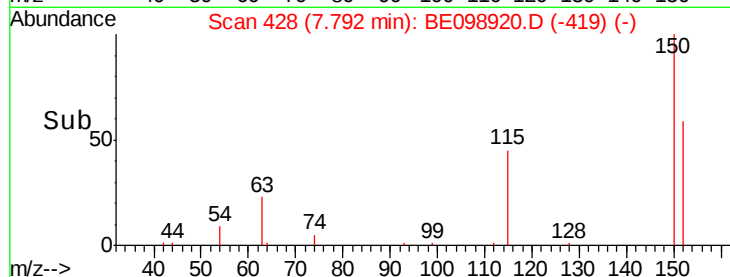


#4

2-Fluorophenol
Concen: 0.146 ng
RT: 5.40 min Scan# 220
Delta R.T. 0.01 min
Lab File: BE098920.D
Acq: 13 Mar 2019 20:15


Tgt Ion:112 Resp: 395
Ion Ratio Lower Upper
112 100
64 83.0 57.9 86.9
63 197.0 158.3 237.5

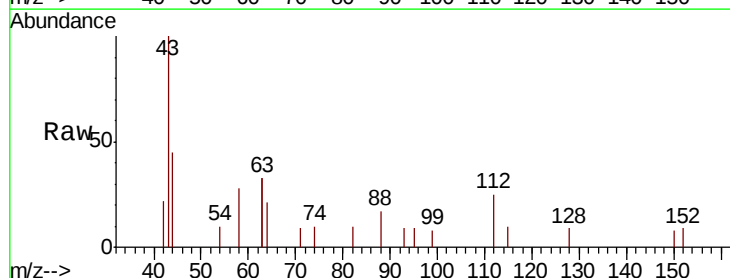


Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

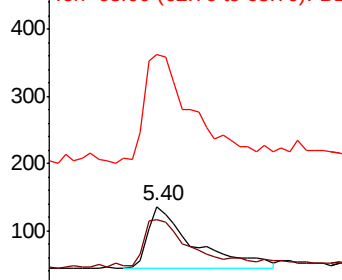

Time-->

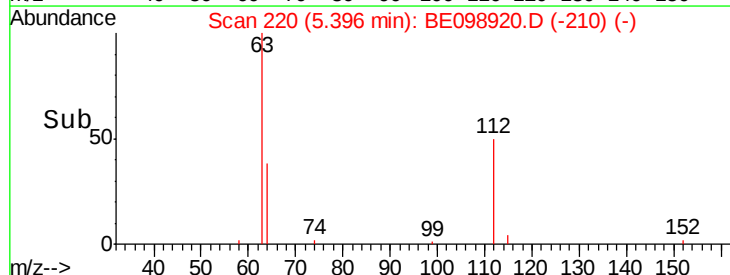

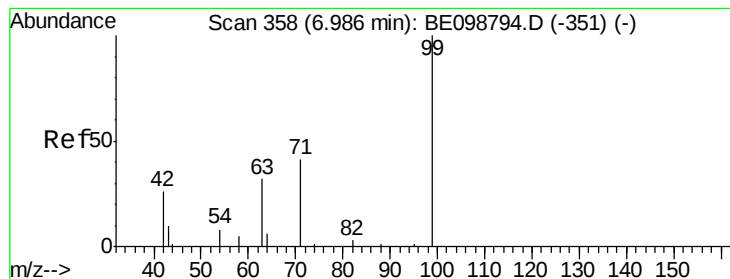

#5

Phenol-d6

Concen: 0.098 ng

RT: 6.99 min Scan# 358

Delta R.T. -0.00 min

Lab File: BE098920.D

Acq: 13 Mar 2019 20:15

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW08-20190311


Tot Ion: 99 Resp: 372

Ion Ratio Lower Upper

99 100

42 47.0 24.2 36.2#


71 40.6 35.7 53.5

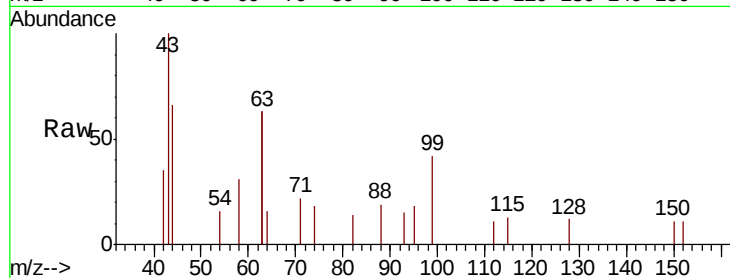



Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

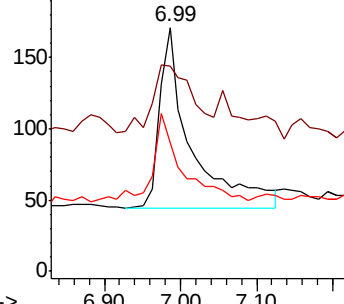

Time-->

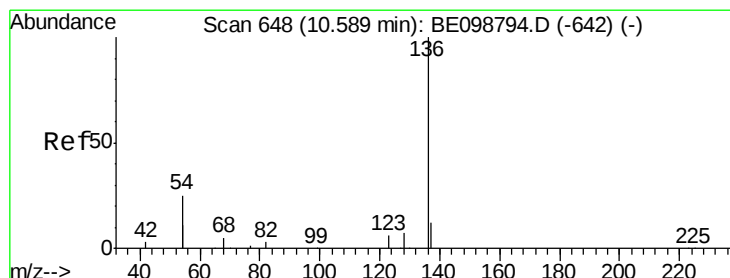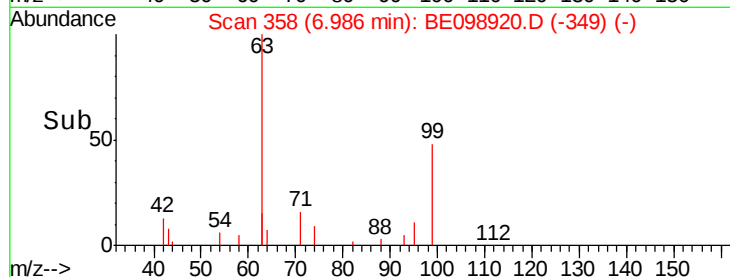

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.59 min Scan# 648

Delta R.T. -0.00 min

Lab File: BE098920.D

Acq: 13 Mar 2019 20:15

Tgt Ion: 136 Resp: 3899


Ion Ratio Lower Upper

136 100

137 13.6 11.4 17.0

54 65.6 39.3 58.9#

68 9.0 6.7 10.1

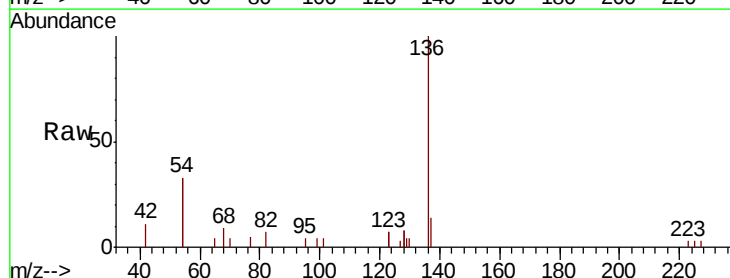


Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

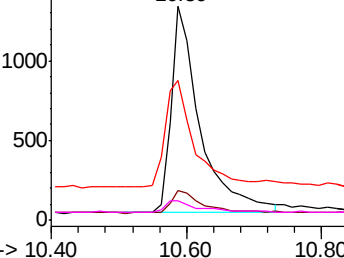

Time-->

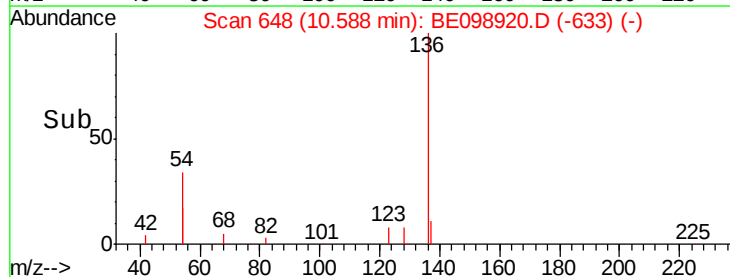



#8

Nitrobenzene-d5

Concen: 0.337 ng

RT: 8.99 min Scan# 525

Delta R.T. 0.03 min

Lab File: BE098920.D

Acq: 13 Mar 2019 20:15

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW08-20190311


Tot Ion: 82 Resp: 1377

Ion Ratio Lower Upper

82 100

128 168.7 123.8 185.8




54 292.5 203.4 305.2

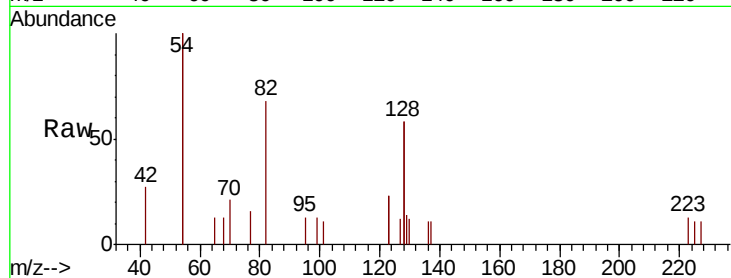

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

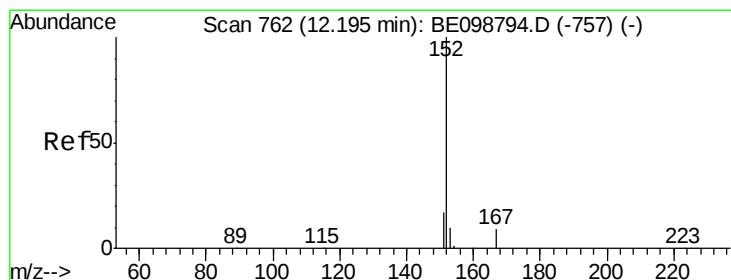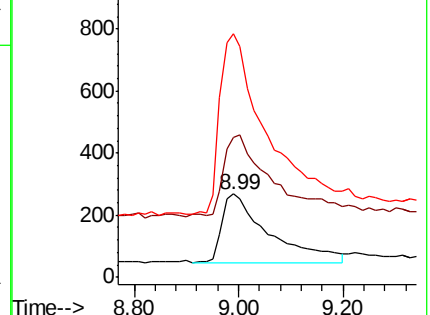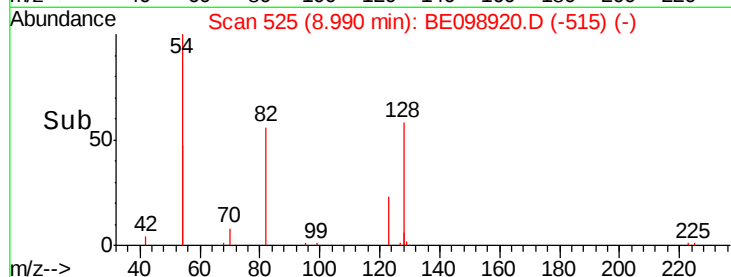

#11

2-Methylnaphthalene-d10

Concen: 0.347 ng

RT: 12.19 min Scan# 762

Delta R.T. 0.00 min

Lab File: BE098920.D


Acq: 13 Mar 2019 20:15

Tgt Ion: 152 Resp: 2501

Ion Ratio Lower Upper



152 100


151 18.4 16.5 24.7

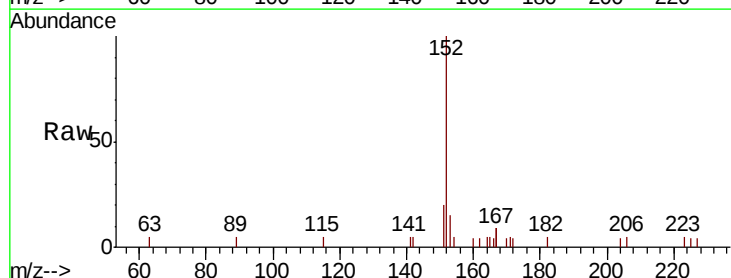

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

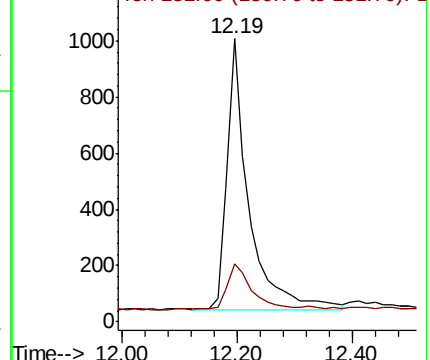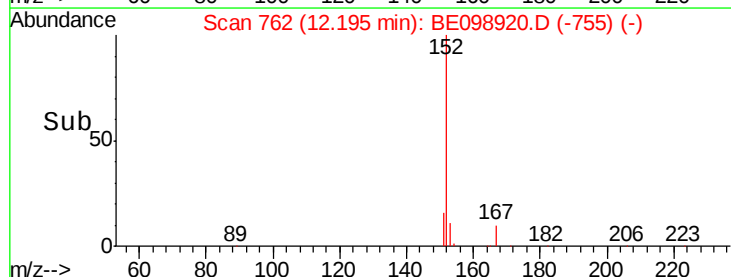


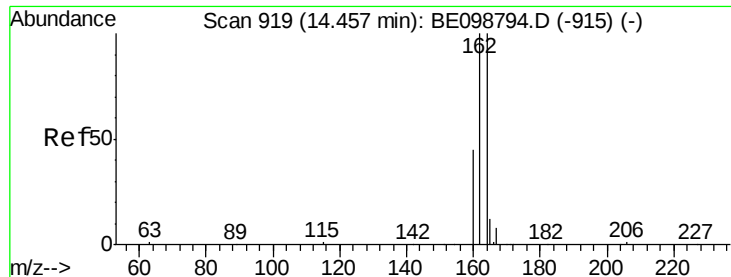




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.46 min Scan# 919
Delta R.T. 0.00 min
Lab File: BE098920.D
Acq: 13 Mar 2019 20:15

Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW08-20190311

Tot Ion:164 Resp: 2765
Ion Ratio Lower Upper
164 100
162 98.5 80.2 120.2
160 47.1 37.8 56.8

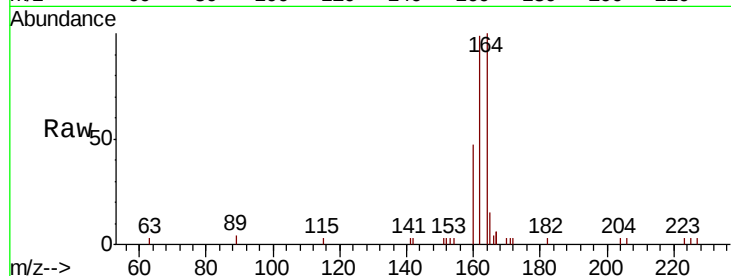


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

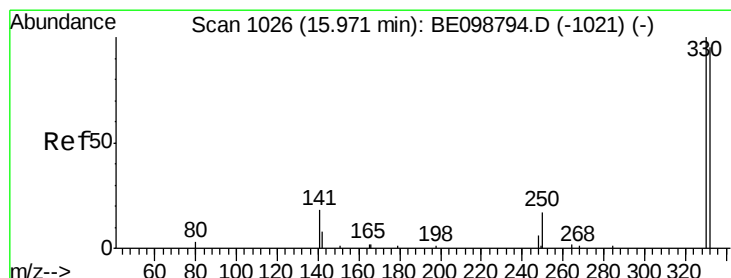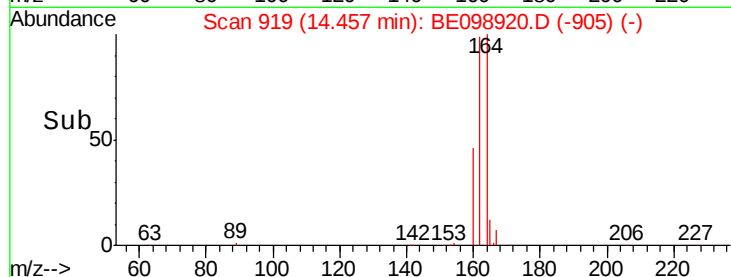
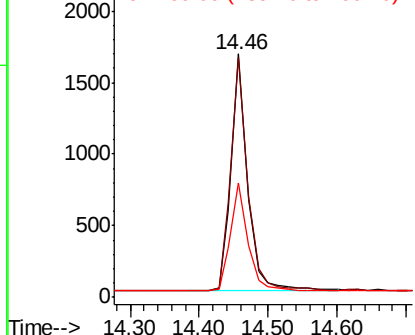



#14
2,4,6-Tribromophenol
Concen: 0.464 ng
RT: 15.96 min Scan# 1025
Delta R.T. -0.01 min
Lab File: BE098920.D
Acq: 13 Mar 2019 20:15

Tgt Ion:330 Resp: 648
Ion Ratio Lower Upper
330 100
332 96.1 77.6 116.4
141 44.0 31.0 46.4

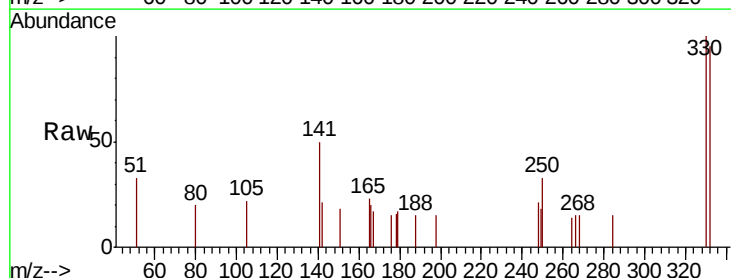

Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



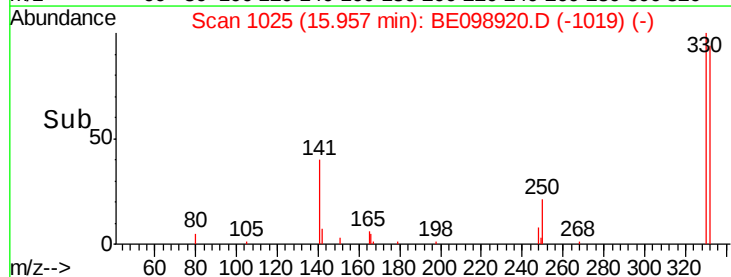
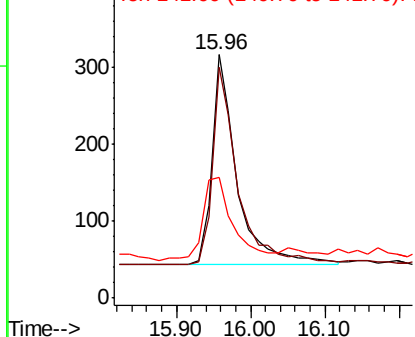


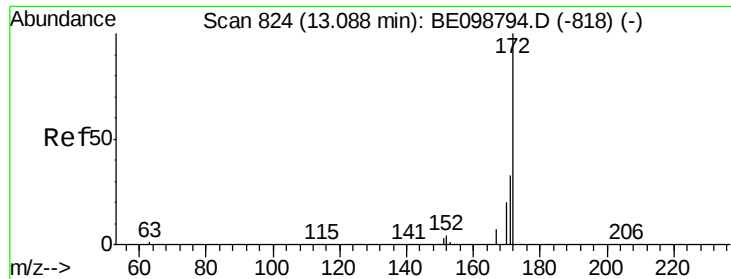

#15
2-Fluorobiphenyl
Concen: 0.758 ng
RT: 13.07 min Scan# 823
Delta R.T. -0.01 min
Lab File: BE098920.D
Acq: 13 Mar 2019 20:15




Instrument :
BNA_E
ClientSampleId :
BP-TT-AOC22-MW08-20190311


Tot Ion:172 Resp: 8676
Ion Ratio Lower Upper
172 100
171 33.0 28.0 42.0
170 23.1 17.7 26.5

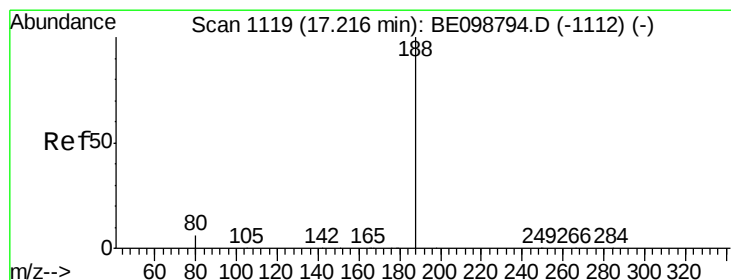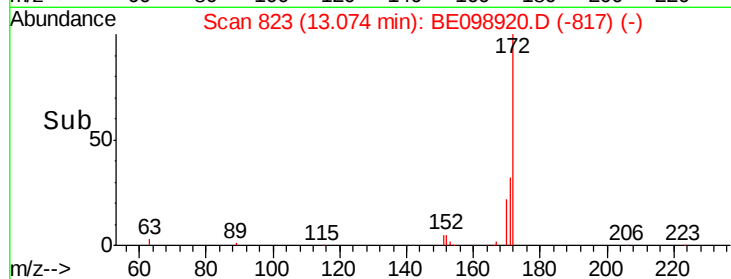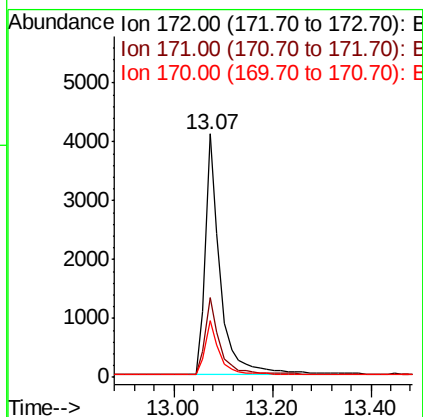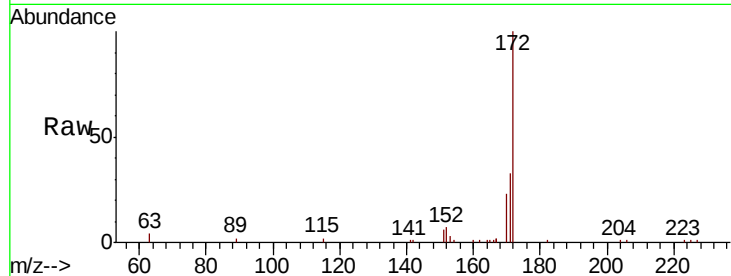

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.22 min Scan# 1119
Delta R.T. -0.00 min
Lab File: BE098920.D
Acq: 13 Mar 2019 20:15

Tgt Ion:188 Resp: 7113
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.5 6.3 9.5

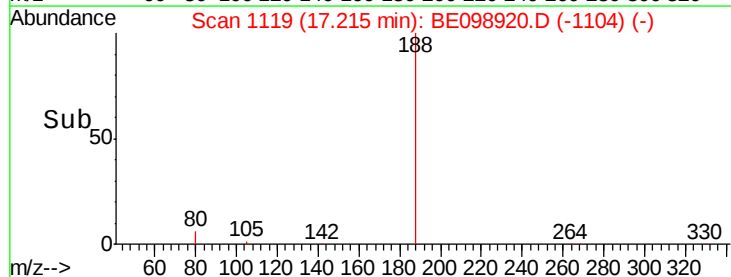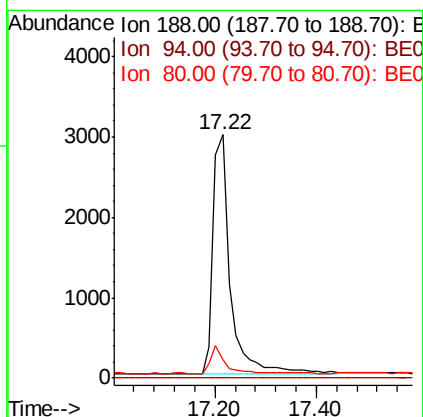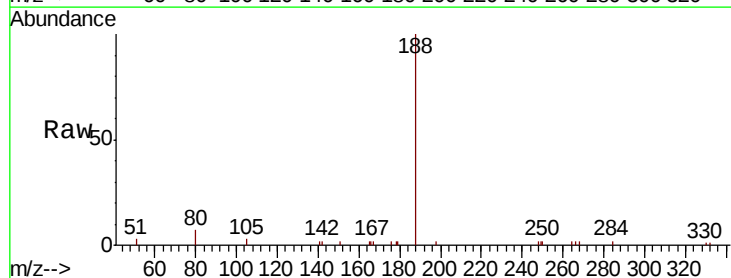

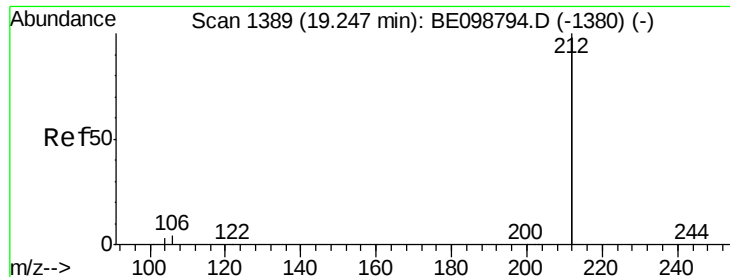

#25

Fluoranthene-d10

Concen: 0.308 ng

RT: 19.24 min Scan# 1388

Delta R.T. -0.01 min

Lab File: BE098920.D

Acq: 13 Mar 2019 20:15


Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW08-20190311




Tot Ion:212	Resp:	34985
Ion Ratio	Lower	Upper
212	100	
106	2.3	1.8 2.8
104	1.5	1.0 1.6

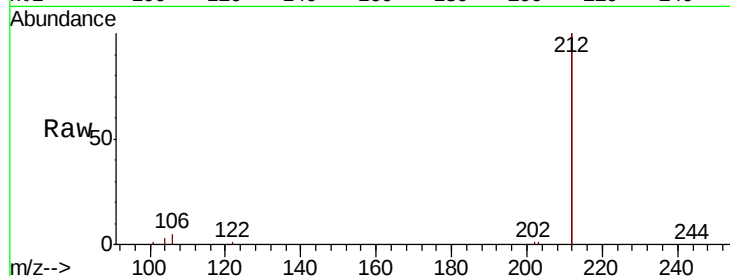

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

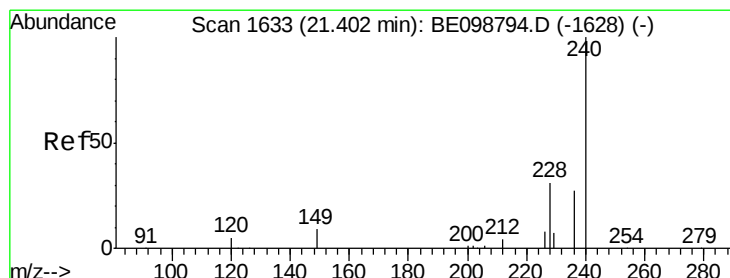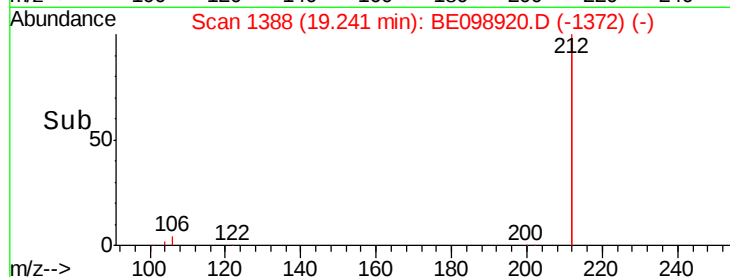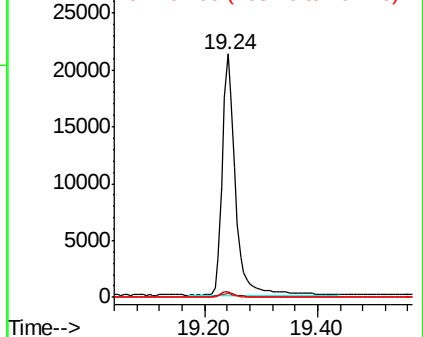

#27

Chrysene-d12

Concen: 0.400 ng


RT: 21.39 min Scan# 1632

Delta R.T. -0.01 min

Lab File: BE098920.D

Acq: 13 Mar 2019 20:15



Tgt Ion:240	Resp:	8090
Ion Ratio	Lower	Upper
240	100	
120	9.2	5.0 7.4#
236	28.2	22.7 34.1

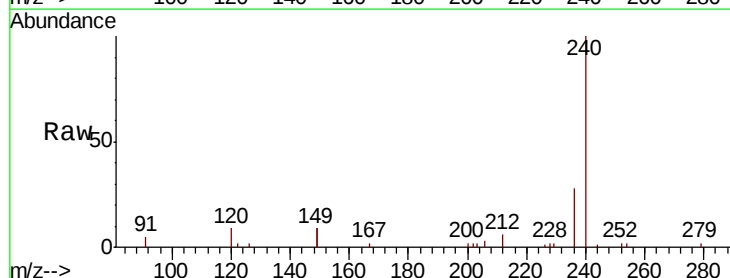


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

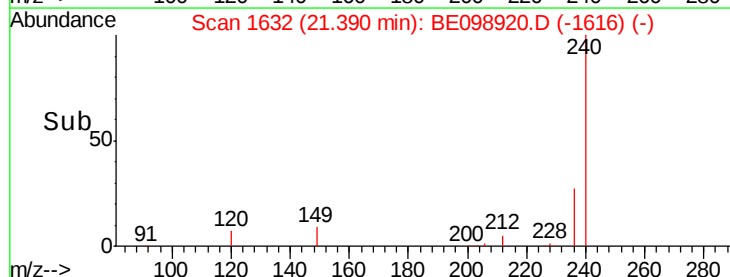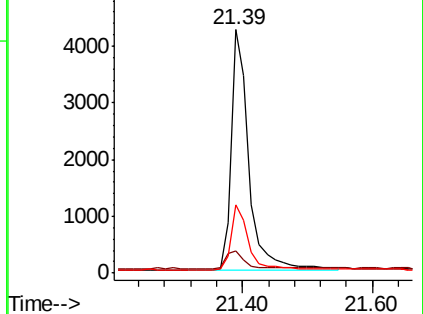

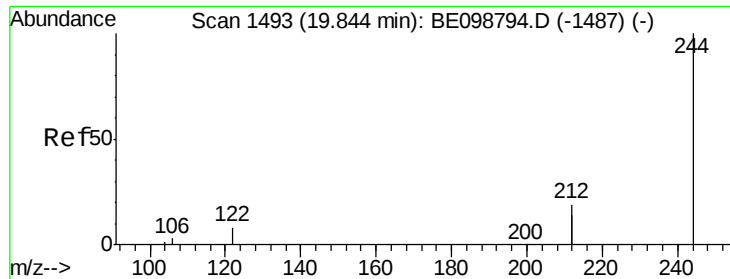

#29

Terphenyl-d14

Concen: 0.499 ng

RT: 19.84 min Scan# 1492

Delta R.T. -0.01 min

Lab File: BE098920.D

Acq: 13 Mar 2019 20:15

Instrument :

BNA_E

ClientSampleId :

BP-TT-AOC22-MW08-20190311


Tot Ion:244 Resp: 9817

Ion Ratio Lower Upper




244 100

212 36.8 29.4 44.2

122 8.4 7.1 10.7

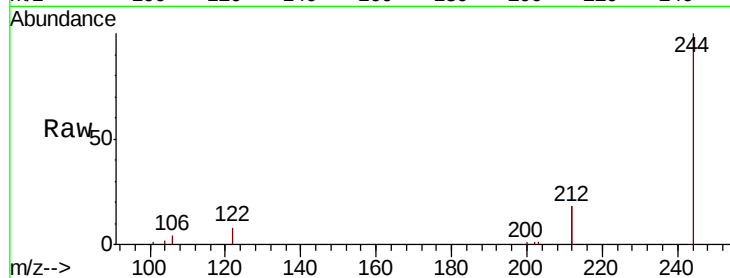

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

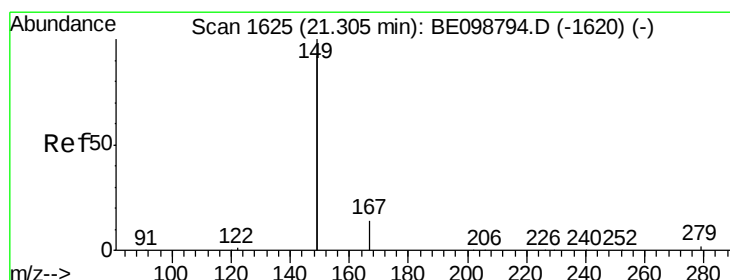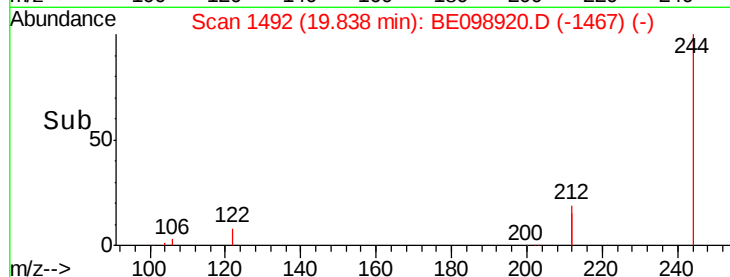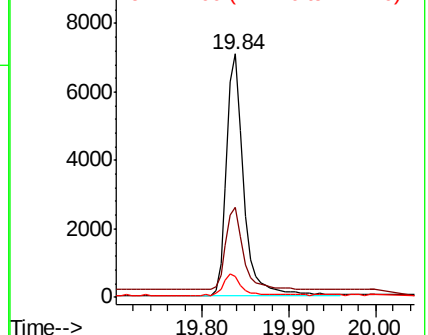

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.079 ng

RT: 21.29 min Scan# 1624

Delta R.T. -0.01 min

Lab File: BE098920.D

Acq: 13 Mar 2019 20:15


Tgt Ion:149 Resp: 4231

Ion Ratio Lower Upper



149 100



167 6.7 5.4 8.0

279 1.9 1.0 1.4#

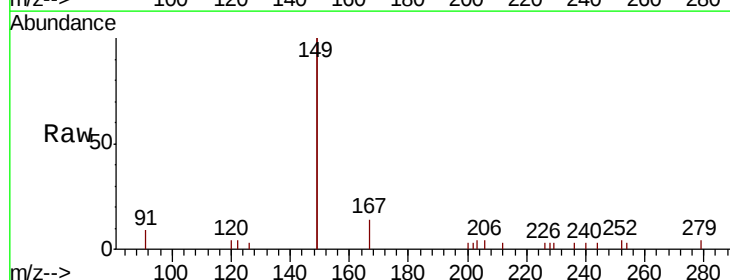

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

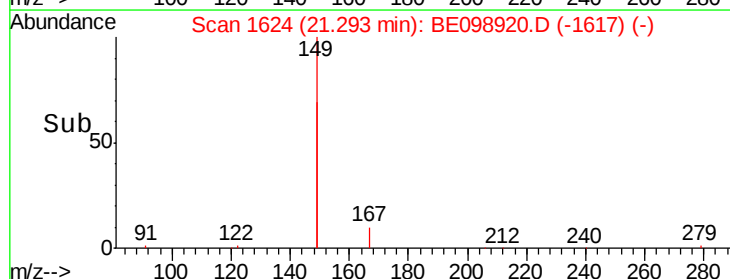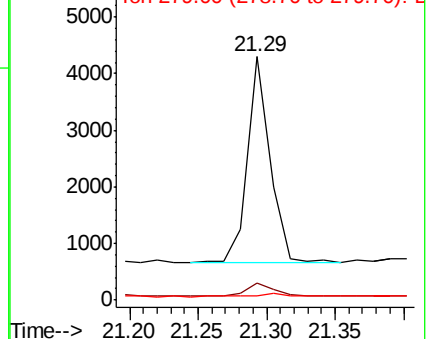

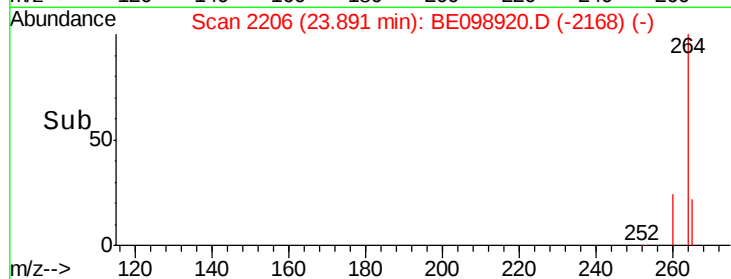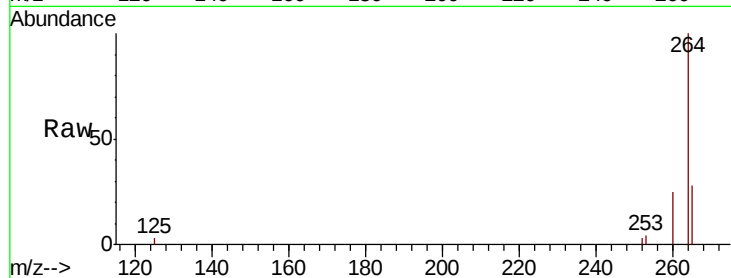

#34
 Pervlene-d12
 Concen: 0.400 ng
 RT: 23.89 min Scan# 2206
 Delta R.T. -0.01 min
 Lab File: BE098920.D
 Acq: 13 Mar 2019 20:15

Instrument :
 BNA_E
 ClientSampleId :
 BP-TT-AOC22-MW08-20190311

Tot Ion:264 Resp: 7882
 Ion Ratio Lower Upper
 264 100
 260 25.1 21.2 31.8
 265 27.5 24.6 36.8

