


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031319\
 Data File : BE098908.D
 Acq On : 13 Mar 2019 11:37
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 06 15:33:24 2019

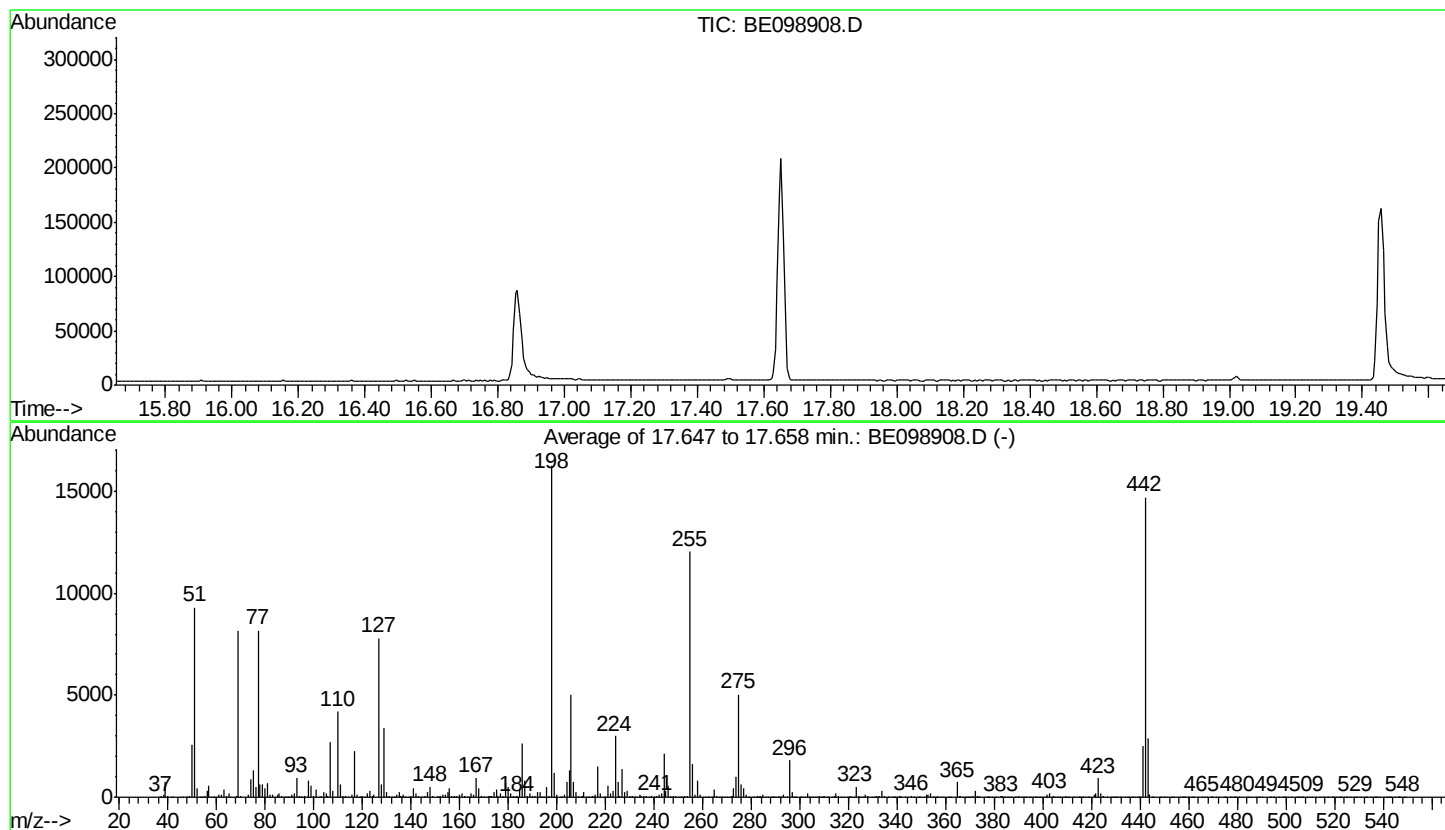

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.3	9318	PASS
68	69	0.00	2	0.5	38	PASS
69	198	0.00	100	50.1	8138	PASS
70	69	0.00	2	0.9	70	PASS
127	198	10	80	48.1	7812	PASS
197	198	0.00	2	0.5	82	PASS
198	198	100	100	100.0	16256	PASS
199	198	5	9	7.2	1173	PASS
275	198	10	60	30.9	5031	PASS
365	198	1	100	4.5	728	PASS
441	198	0.01	100	15.4	2500	PASS
442	198	50	100	90.5	14710	PASS
443	442	15	24	19.6	2887	PASS