


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE031319\
 Data File : BE098924.D
 Acq On : 13 Mar 2019 23:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE030619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 06 15:33:24 2019

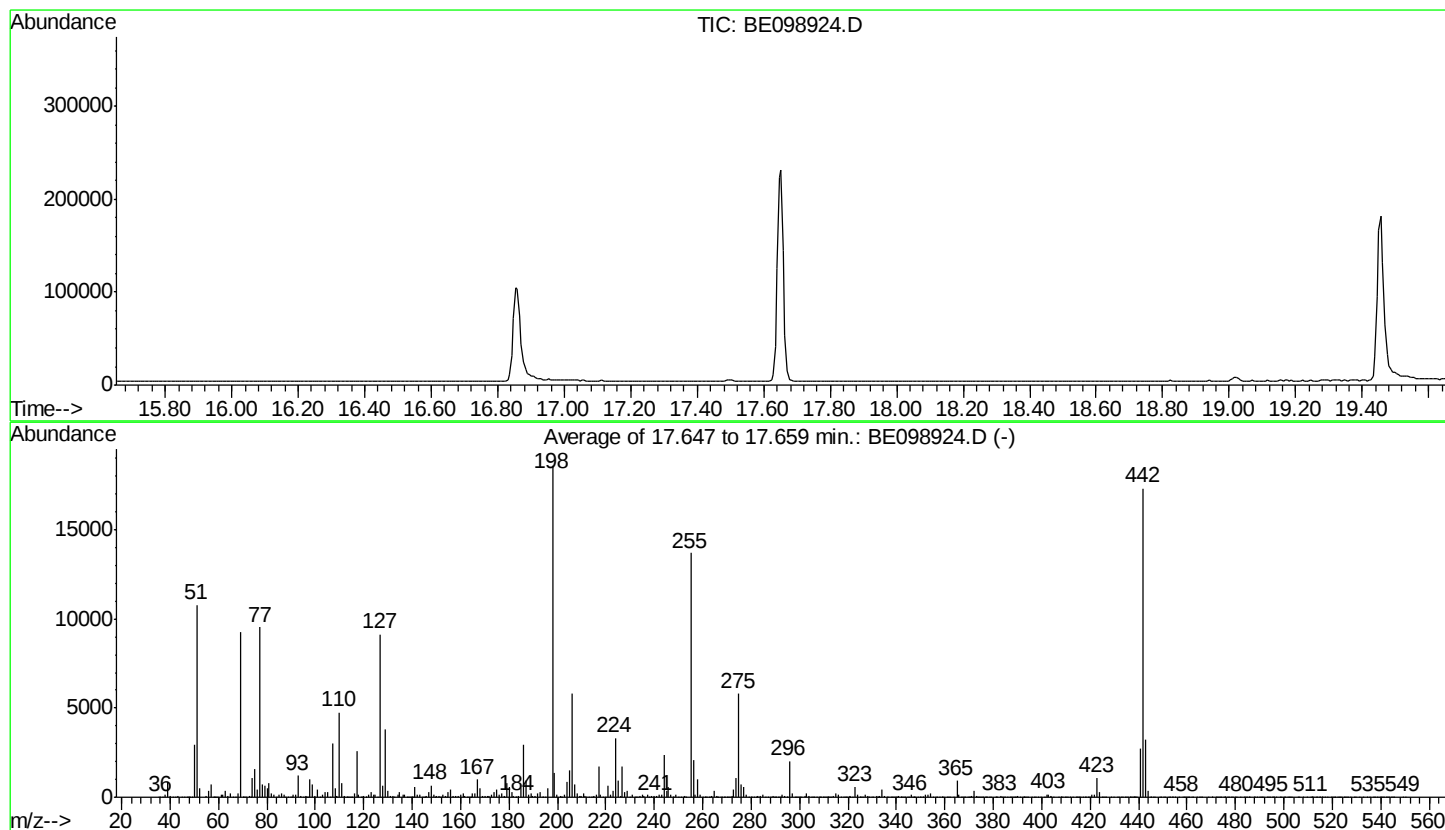

AutoFind: Scans 2563, 2564, 2565; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.0	10795	PASS
68	69	0.00	2	2.0	187	PASS
69	198	0.00	100	50.0	9294	PASS
70	69	0.00	2	0.2	14	PASS
127	198	10	80	49.2	9153	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18597	PASS
199	198	5	9	7.2	1342	PASS
275	198	10	60	31.1	5786	PASS
365	198	1	100	4.9	917	PASS
441	198	0.01	100	14.8	2744	PASS
442	198	50	100	93.2	17337	PASS
443	442	15	24	18.8	3260	PASS