
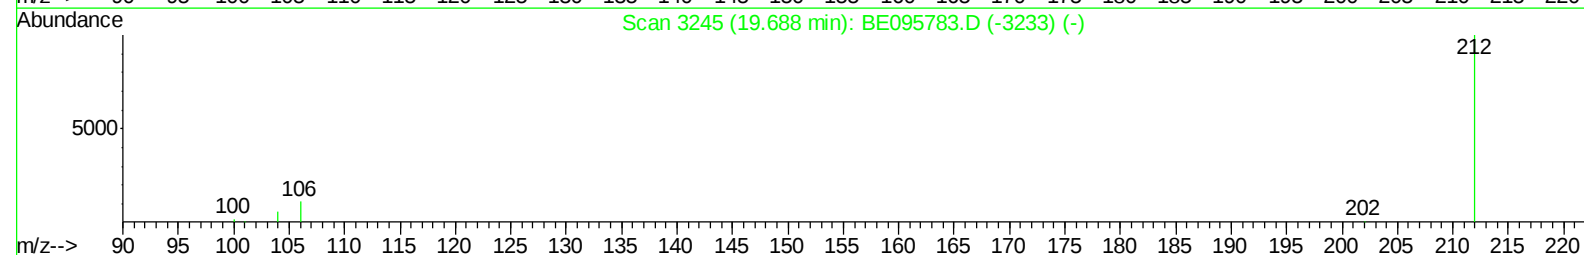
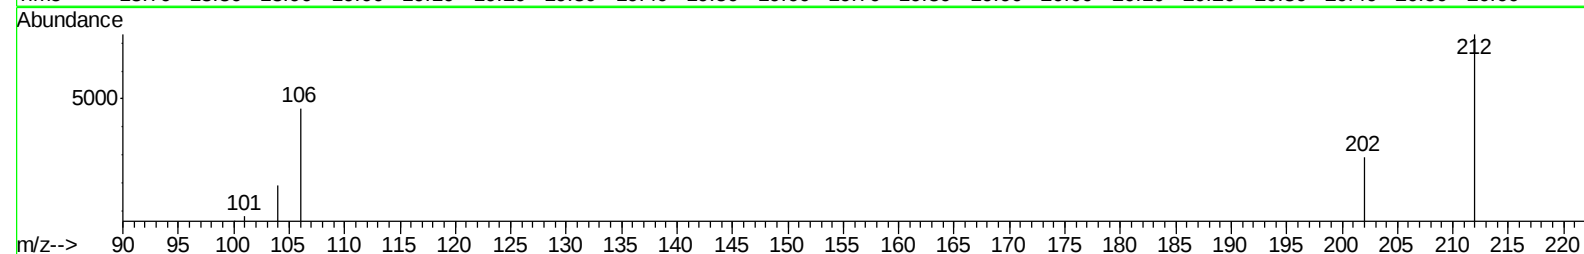


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\
Data File : BE095788.D
Acq On : 15 Mar 2018 5:32
Operator : SJ/JU
Sample : J1835-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Mar 15 08:44:35 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 15 05:35:28 2018
Response via : Initial Calibration

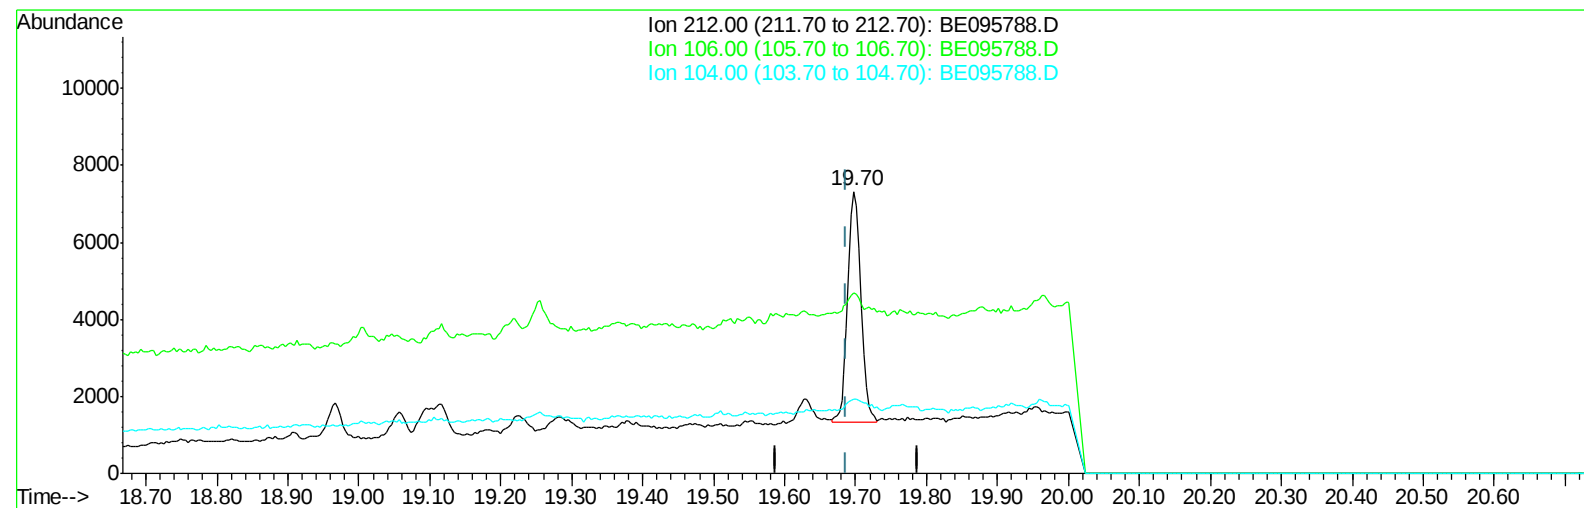

TIC: BE095788.D

(14) Fluoranthene-d10 (SURR)

19.698min (+0.010) 0.25ng/ul m

response 7804

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.70#
104.00	15.60	0.78#
0.00	0.00	0.00