
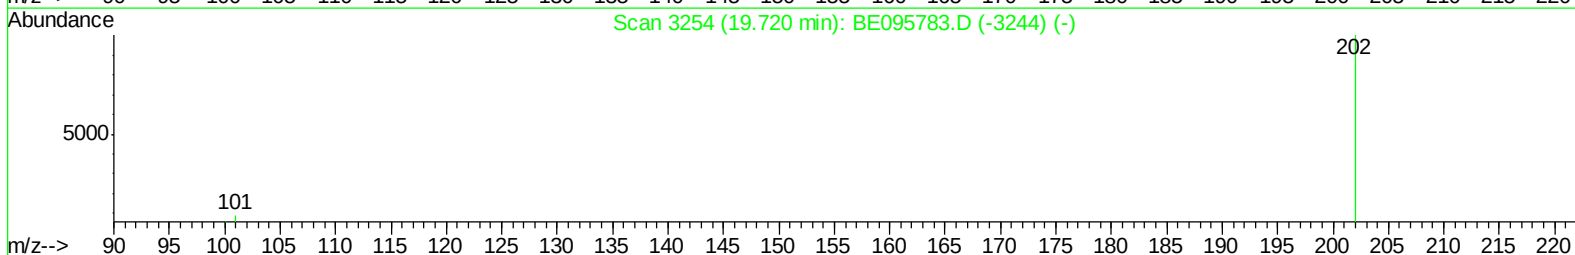
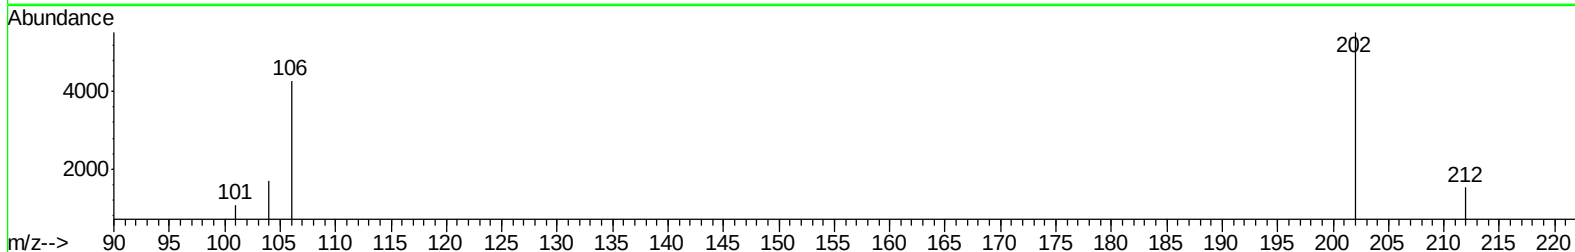


Data Path : Z:\HPCHEM1\BNA E\DATA\BE031418\  
Data File : BE095788.D  
Acq On : 15 Mar 2018 5:32  
Operator : SJ/JU  
Sample : J1835-15  
Misc :  
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Mar 15 08:44:35 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE031318.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 15 05:35:28 2018  
Response via : Initial Calibration

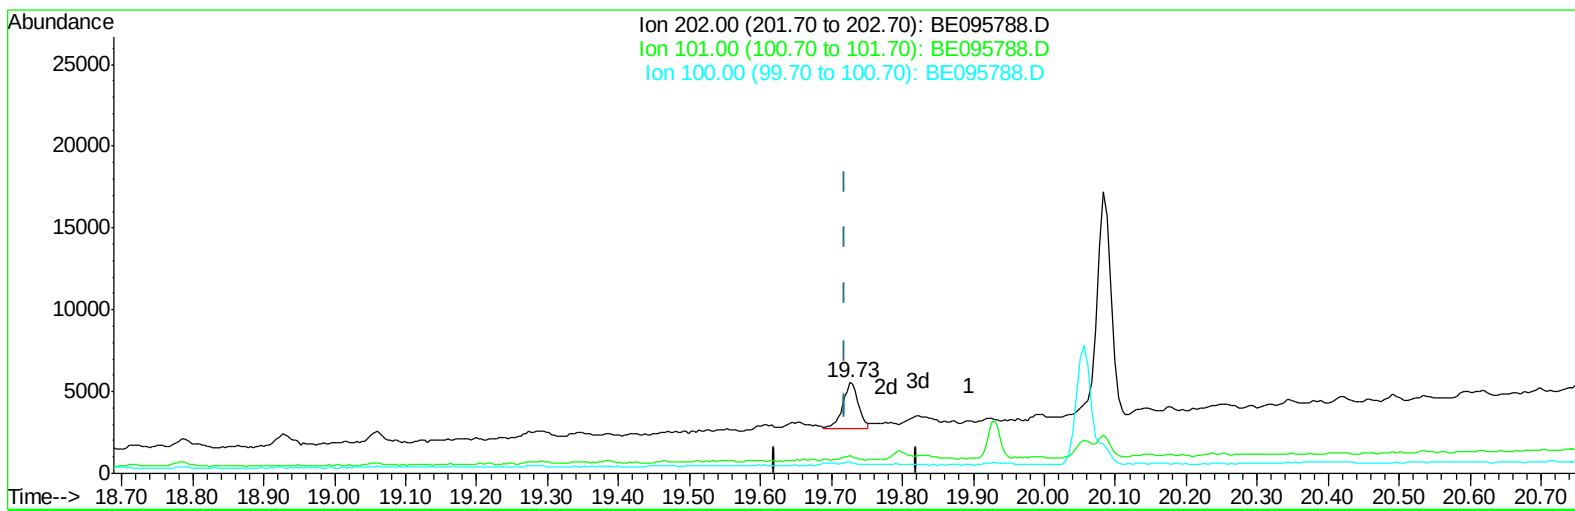

TIC: BE095788.D

(15) Fluoranthene (C)

19.727min (+0.007) 0.12ng/ul m

response 4206

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 202.00 | 100   | 100   |
| 101.00 | 10.30 | 19.23 |
| 100.00 | 19.50 | 12.49 |
| 0.00   | 0.00  | 0.00  |